

Florida Department of Environmental Protection



2021 Annual Ambient Air Monitoring Network Plan

**Division of Air Resource Management
Florida Department of Environmental Protection
June 2021**

TABLE OF CONTENTS

1.0 INTRODUCTION	1
2.0 AIR MONITORING NETWORK 2021	3
2.1 Network Design Principles	3
2.2 Network Equipment Upgrades and Enhancement.....	5
3.0 AIR MONITORING NETWORK MODIFICATIONS	7
3.1 Site Shut-downs, Set-ups and Relocations	9
<i>A. Site Shut-downs</i>	9
<i>B. Site Relocations</i>	12
4.0 FLORIDA'S AMBIENT AIR MONITORING NETWORK 2019.....	14
4.1 Ozone Network.....	14
4.2 PM _{2.5} Network	16
4.3 NCore Network.....	18
4.4 PAMS NETWORK	19
4.5 NATTS Network	22
4.6 SO ₂ Monitoring Network.....	23
4.7 NO ₂ Monitoring Network.....	26
4.8 CO Monitoring Network	30
4.9 PM ₁₀ Monitoring Network.....	31
4.10 Lead Monitoring Network	33
5.0 MONITORING WAIVERS.....	34
6.0 GLOSSARY OF AIR MONITORING TERMS	43
7.0 APPENDICES	44
Appendix A: Additional Network Information	44
<i>A.1 Site Relocations</i>	44
<i>A.2 Temporary Discontinuance</i>	51
Appendix B: Annual Site Review Summary	56
Appendix C: Ambient Air Monitoring Network Description	63
Appendix D: Ambient Air Monitoring Inventory	71

LIST OF FIGURES

Figure 1.1 2021 Site Locations for Florida's Ambient Air Monitoring Network	1
Figure 4.1 2019 Crude Rate of Asthma hospitalizations, Rate Per 100,000 Population	28
Figure 5.2 Street View of Woodlawn	40
Figure 5.3 East of Woodlawn Site	40
Figure 6.1 North from Proposed Wittkop Park Site	44
Figure 6.2 South from Proposed Wittkop Park Site	45
Figure 6.3 East from Proposed Wittkop Park Site.....	45
Figure 6.4 West from Proposed Wittkop Park Site.....	46
Figure 6.5 Aerial of Proposed Wittkop Park Site	46
Figure 6.6 Wind Rose from Wittkop (AQS Site 12-086-6002).....	47
Figure 6.7 North from Proposed Winter Park Site	48
Figure 6.8 East from Proposed Winter Park Site.....	48
Figure 6.9 South from Proposed Winter Park Site	49
Figure 6.10 West from Proposed Winter Park Site.....	49

LIST OF TABLES


Table 1.1 Florida's Primary Quality Assurance Organization	2
Table 2.1 Equipment Purchases 2020	5
Table 3.1 Summary of Network Modifications	7
Table 3.2 Site and Monitor Evaluation Summaries for Discontinuation.....	9
Table 3.3 40 CFR Part 58.14(c) and Ambient Air Monitoring Network Assessment Guidance Calculations.....	10
Table 3.4 Homestead Fire Station - AQS Site # 12-086-6001	11
Table 4.1 Florida's Ozone Network.....	14
Table 4.2 Florida's PM _{2.5} Network	16
Table 4.3 NCORE Sites in Florida	18
Table 4.4 NATTS Sites in Florida	22
Table 4.5 SO ₂ Monitoring Requirements.....	23
Table 4.6 Florida's SO ₂ Network.....	25
Table 4.7 NO ₂ Monitoring Required by 2010 NAAQS.....	27
Table 4.8 Florida's NO ₂ Near-road Network and Monitor Designations	29
Table 4.9 Florida's CO Network	30
Table 4.10 Florida's PM ₁₀ Network.....	31
Table 4.11 Florida's Lead Source Monitoring Network.....	33
Table 5.5 2020 Site Review of Woodlawn - AQS Site #12-103-0012	39

1.0 INTRODUCTION

The Florida Department of Environmental Protection (DEP) has developed and maintains a comprehensive ambient air monitoring network that covers over 90 percent of the 21 million people living in Florida, the third most populous state in the United States. This network is designed to provide the public with accurate air quality information, and currently meets or exceeds federal air monitoring requirements.

The network is comprised of more than 177 monitors at 90 sites strategically positioned across the state. As shown in Figure 1.1, these sites are concentrated in areas of higher population density, along the coast, and near interstate highways. In addition, the Department established three rural monitoring sites as representative locations for comparison to regional background levels of pollution: one in the panhandle, one in the northern area of the peninsula, and one in the southern area of the peninsula.

Figure 1.1 2021 Site Locations for Florida's Ambient Air Monitoring Network

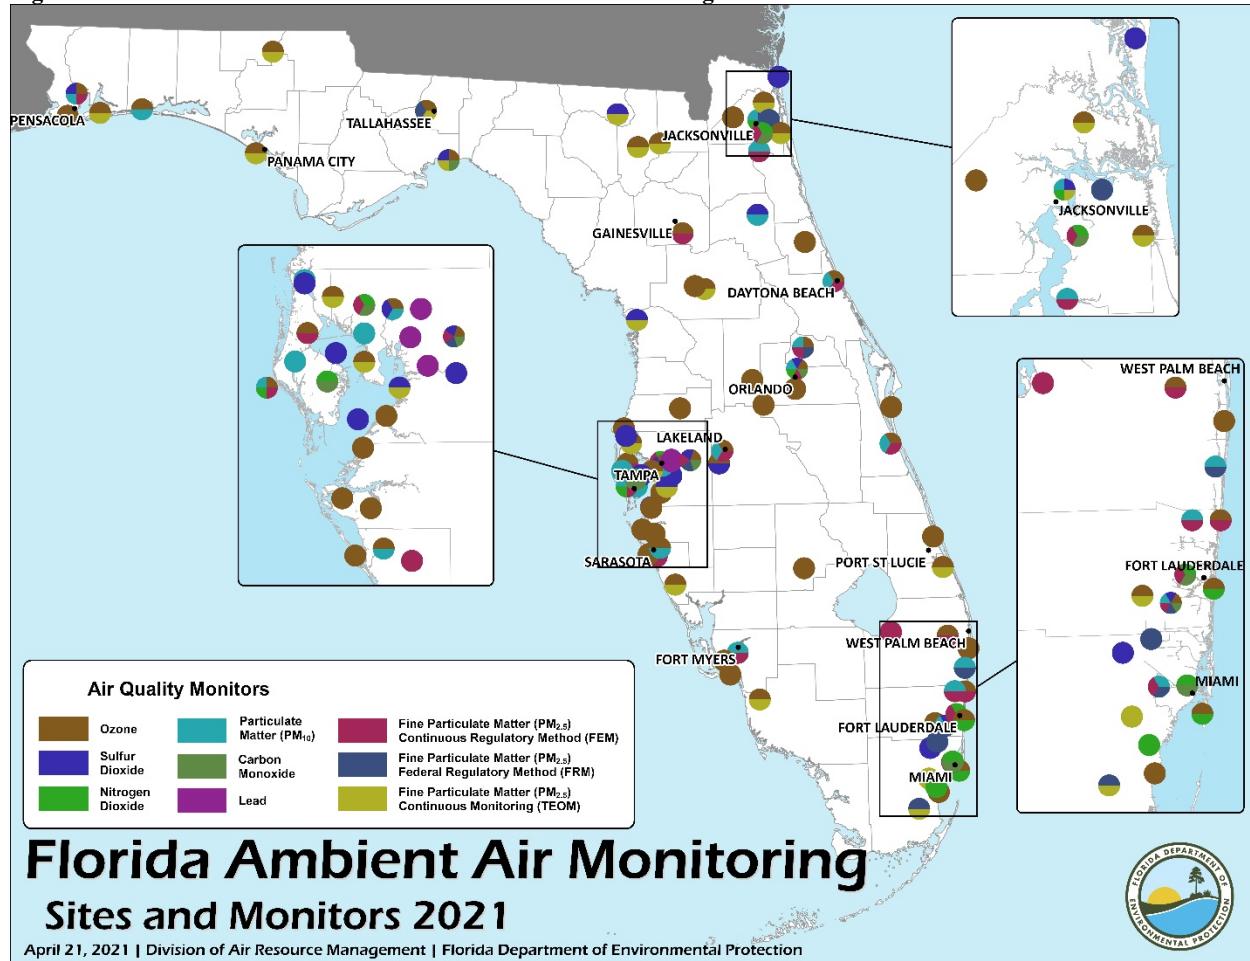

All of Florida's monitoring agencies are managed under a Primary Quality Assurance Organization (PQAO) to ensure that monitoring is conducted according to a common set of procedures, using common calibration facilities and standards, and with oversight by a single air quality agency. DEP's Division of Air Resource Management is the coordinating agency that oversees this PQAO, which consists of DEP and nine Local Programs (see Table 1.1 below).

Table 1.1 Florida's Primary Quality Assurance Organization

DEP's Division of Air Resource Management	Local Programs
Office of Air Monitoring	Broward County
Emerald Coast (Panama City area)	City of Jacksonville
First Coast (Jacksonville area)	Hillsborough County
Forgotten Coast (Tallahassee area)	Manatee County
Lee Island Coast (Ft. Myers area)	Miami-Dade County
Nature Coast (Gainesville area)	Orange County
Naval Aviation Coast (Pensacola area)	Palm Beach County
Space Coast (Orlando area)	Pinellas County
Sun Coast (Tampa area)	Sarasota County

Florida's air monitoring network is designed to provide timely air pollution data to the public, support compliance with ambient air quality standards, develop emission reduction strategies, and support air pollution research studies. Data gathered from Florida's monitoring network are used to:

- Determine an area's compliance with the National Ambient Air Quality Standards (NAAQS);
- Produce a daily Air Quality Index (AQI) report;
- Compile daily air quality forecast reports;
- Support short and long-term health risk assessments;
- Identify localized health concerns; and
- Track long-term trends in air quality that could potentially affect the quality of life of Florida's residents and visitors.

This annual Air Monitoring Network Plan is a requirement of the Code of Federal Regulations (40 CFR 58) established by the U.S. Environmental Protection Agency (EPA). The purpose of this report is to provide evidence that Florida's air monitoring network meets current regulations, detail any changes proposed for the 18 months following its publication, and provide specific information on each of the state's existing and proposed monitoring sites. Federal regulations require that the plan be posted for public comment 30 days before submission to the EPA Regional Office. The plan was made available to the public on the DEP website from May 21, 2021, through June 20, 2021, for the 30-day comment period.

2.0 AIR MONITORING NETWORK 2021

On January 1, 2015, the U.S. Environmental Protection Agency (US EPA) designated the State of Florida as one Primary Quality Assurance Organization (PQAO) responsible for monitoring air pollution. Florida's PQAO consists of Florida DEP as the lead agency and 9 local air monitoring organizations throughout the state. Florida's air monitoring network is critical for assessing the state's progress in maintaining and improving air quality, understanding temporal variations in air pollutants, and evaluating pollutant exposure by individuals and the environment. One fundamental purpose of monitoring is to distinguish between areas where pollutant levels violate the ambient air quality standards and areas where they do not. Areas in violation of a standard require increased efforts to reduce the pollution that results in exceedances. Air quality agencies develop strategies, programs, and regulations to achieve needed emission reductions. Data from Florida's air monitoring network are then used to determine the rate of progress toward attaining the standards.

DEP will submit the 2021 Annual Air Monitoring Network Plan to EPA on June 29, 2021, for review and approval.

2.1 NETWORK DESIGN PRINCIPLES

The principles that guide Florida's network design are:

1. Sites will meet the Code of Federal Regulations for the number, type, and placement of monitors.
2. Attention will be paid to historic areas of exceedances or violations where contributing industries, activities, and/or populations have been maintained.
3. There will be sufficient ozone and fine particle pollution monitors to maintain AQI reporting for large (350,000+ population) communities.
4. During network design, the weight will be given to monitors that have long historical records.
5. Partnerships with private entities will be used judiciously.
6. Any monitoring required by the State Implementation Plans (SIP) will continue.
7. Coordination with Florida's local programs will be maintained to achieve a quality statewide network.

Details of the network are in the "Network Description and Requirements" section of this plan. The network description is organized first by the largest Metropolitan Statistical Areas followed by the monitoring of areas, not within a Metropolitan Statistical Area. Nine county agencies assist DEP in the operation of the statewide air monitoring network. Each county's Metropolitan Statistical Areas or Micropolitan Statistical Area is identified. Requirements for the minimum number of monitoring sites are dependent on both population and population concentration for ozone, PM_{2.5}, and PM₁₀. The recently calculated Population Weighted Emission Index (PWEI) is listed for any areas with a PWEI over 5,000 where monitoring for sulfur dioxide is required.

The Air Quality Index (AQI) is reported and updated hourly on DEP's website at www.floridadep.gov/air/air-monitoring/content/floridas-air-quality. It is available in both graphical and text versions. The data to support this website are collected from all continuous monitors in the state. These data are also shared on EPA's AIR NOW site at www.airnow.gov.

An Air Monitoring Network Plan is also required to provide evidence that siting and operation of each monitor meet the requirements of Appendices A, B, C, D, and E of 40 CFR Part 58, where applicable. Appendix A specifies the minimum quality system requirements applicable to State and Local Air Monitor Stations (SLAMS) and other monitor types whose data are intended to be used to determine compliance with NAAQS. Florida meets 40 CFR Part 58, Appendix A requirements with three basic functions:

1. A quality system must have approved standard operating procedures (SOP), a Quality Management Plan (QMP), and Quality Assurance Project Plans (QAPP), which are in place and updated as needed. The Gaseous QAPP was approved in November 2019 and the PM_{2.5} QAPP was approved in October 2020. The current QMP was approved in June 2019.
2. DEP Quality Assurance staff complete instrument performance and technical systems audit for all agencies throughout the state.
3. All quality assurance and quality control records must be sent to EPA's Air Quality System (AQS) database quarterly.

40 CFR Part 58, Appendix B, describes quality assurance requirements for Prevention of Significant Deterioration (PSD) air monitoring. Florida's air monitoring network does not include any PSD monitors; therefore, these requirements are not applicable.

40 CFR Part 58, Appendix C, describes general ambient air quality monitoring methodology. Florida's air monitoring network is comprised of both federally and non-federally approved instrumentation. Only data from the federally approved instrumentation can be used for designations. Additionally, all instruments are subjected to the same quality assurance and quality control requirements as those used for designations. Florida's instrumentation meets 40 CFR Part 58, Appendix C requirements and is described in detail in Appendix C of this Plan.

40 CFR Part 58, Appendix D, contains the network design criteria for ambient air quality monitoring. Sites within Florida's air monitoring network are established using these requirements. This annual Air Monitoring Network Plan assesses the network's ability to meet these requirements.

40 CFR Part 58, Appendix E, contains the probe siting criteria for ambient air quality monitoring. To assure that these requirements continue to be met, sites are reviewed annually by DEP QA audit staff. The results of these reviews are used to determine if the sites meet siting requirements. Any discrepancies are dealt with, at minimum, on an annual basis. A table summarizing the site reviews conducted in the last year, as well as any issues discovered, is provided in Appendix B of this Plan. All of Florida's sites meet 40 CFR Part 58, Appendix E unless explicitly noted in Appendix B of this Plan.

2.2 NETWORK EQUIPMENT UPGRADES AND ENHANCEMENT

Over the last several years, the PQAO has made extensive investments into Florida's air monitoring network. These upgrades and enhancements have been implemented to take advantage of software and hardware technological advancements for greater operational efficiency. These equipment upgrades are reflected in the "Network Description and Requirements" and "Network Equipment Evaluation" sections of the plan. The following, Table 2.1, are major equipment purchases and upgrades accomplished during the last 18 months:

Table 2.1 Equipment Purchases 2020

Agency	Quantity	Equipment Purchases
DEP	2	49IQPS Calibrators
DEP	2	49IQ Analyzers
DEP	1	T640X Analyzer
DEP	5	8872 Data Loggers
Broward County	1	Teledyne T640
Broward County	1	ESC 8872
Broward County	1	Teledyne T700U
Broward County	1	Teledyne T400
Broward County	1	Teledyne T703
Broward County	1	RM Young 52203
Broward County	1	RM Young 41342VC
Broward County	1	RM Young 61402V
Broward County	1	Teledyne API, T500U
Broward County	1	Thermo 42i-Y
Broward County	1	CAS turn-key Chromatotec AutoGC-FID, M41022
Broward County	1	Kipp & Zonen SMP6-V
Broward County	1	Kipp & Zonen SUV5-V
City of Jacksonville	2	Thermo 111iQ Zero Air Generators
City of Jacksonville	2	Teledyne T700U Calibrators
City of Jacksonville	1	Teledyne T640
Hillsborough County	1	RM Young Ultrasonic Anemometer
Hillsborough County	2	Thermo TEOM 1405 Continuous Ambient Particulate Monitors
Hillsborough County	1	Thermo Fisher 42i-Y
Hillsborough County	2	Thermo Fisher 1405
Hillsborough County	1	TSI EPC3783
Hillsborough County	1	Magee AE-33
Hillsborough County	1	Thermo Fisher 48iQ-TLE
Hillsborough County	1	Thermo Fisher 43iQ
Hillsborough County	1	Thermo Fisher 5014i
Hillsborough County	1	Thermo Fisher 49iQ
Hillsborough County	1	Thermo Fisher 49iQ PS
Hillsborough County	1	Teledyne T200UP
Hillsborough County	4	DIY Zero Air Systems

Manatee County	1	Shelter (39th)
Manatee County	1	Barometer
Manatee County	3	Airlink MG90
Miami-Dade County	1	API Teledyne T701H
Miami-Dade County	1	API Teledyne T200
Miami-Dade County	1	API Teledyne T700U
Miami-Dade County	3	TEI 49iQ
Miami-Dade County	2	TEI 43iQ
Miami-Dade County	1	Teledyne T640 w/ outdoor enclosure
Miami-Dade County	2	TEI 2025i Samplers
Orange County	1	Nikon Forestry Pro II Laser Rangefinder
Orange County	1	MesaLabs Flexcal
Palm Beach County	1	Teledyne 640x Shelter
Palm Beach County	1	Server
Palm Beach County	2	Agilaire 8872 datalogger
Pinellas County	2	Teledyne API T400- Ozone analyzer
Pinellas County	1	Teledyne API T500U - NO2 analyzer
Pinellas County	1	Teledyne API T700U - Dynamic dilution calibrator
Pinellas County	1	Teledyne API T640 - PM2.5 FEM monitor
Pinellas County	7	4G Cellular Routers
Pinellas County	7	Digital internal shelter temperature units
Sarasota County	3	Agilaire 8872 Data Loggers

3.0 AIR MONITORING NETWORK MODIFICATIONS

This Air Monitoring Network Plan lists the known changes to the network that have occurred in the last 18 months and those expected to occur in FY 2021. The discussion within this plan is organized as follows:

- Sites scheduled to shut down, set-up, or relocate;
- Scheduled monitor changes and discontinuations; and
- Network descriptions organized by pollutant for 2021.

This plan also provides additional site information in Appendix A, a summary of all site reviews for the network in Appendix B and a complete inventory list in Appendix C. DEP reserves the right to make unplanned network changes in the event a site needs to be closed or relocated due to events beyond our control, and will communicate these unforeseen events to the USEPA. These may include but are not limited to, issues with site access and unpredictable circumstances. Significant network modifications for 2021 are provided in Table 3.1.

Table 3.1 Summary of Network Modifications

AQS Site #	Site Name	Parameter	Modification
12-011-0033	Vista View Park	PM _{2.5}	Replacement of SPM MET One BAM 1020 with SLAMS T640 FEM monitor relocated from Coconut Creek (12-011-5005). SU EXPECTED 10/2021
12-011-5005	Coconut Creek	PM _{2.5} , PM ₁₀	Replacement of PM ₁₀ MET One eBAMS+ with T640X. SU EXPECTED 10/2021 Replacement of PM _{2.5} T640 with T640X. SU EXPECTED 10/2021 Relocation of T640 to Vista View Park (12-011-0033).
12-031-0081	Cedar Bay STP	SO ₂	Closed 3/2021. Source monitoring site, Cedar Bay Generating Plant. The plant shut down in 2016.
12-031-0099	Sunny Acres	PM2.5	A shutdown of Manual 2025i samplers. SD EXPECTED 09/2021 Addition of Continuous T640 FEM sampler. SU EXPECTED 10/2021
12-031-0108	Pepsi Place	PM2.5, CO, NO ₂	Scheduled to shut down due to construction of a ramp in the location as early as Summer 2023. Proposed concurrent study of NO ₂ at the Roselle testing site or other proposed location to take place in 2022
12-033-0044	Ellyson Industrial Park	PM _{2.5} , PM ₁₀	Replace PM _{2.5} Teledyne T640 with T640X. Add PM ₁₀ Teledyne T640X monitor. SU 02/2021
12-071-0005	Winkler Pump Station	PM _{2.5} , PM ₁₀ , O ₃	Replace PM10 Thermo 1405, and Teledyne T640 with collocated T640X monitors. SU EXPECTED 06/2021 Add/Relocate 49i monitor from Bay Oaks Park (12-071-3002). SU EXPECTED 05/2021
12-071-3002	Bay Oaks Park	O ₃	Temporary relocation due to park construction SD EXPECTED 05/2021.

			Working with EPA to determine permanent highest concentration ozone site.
12-081-4012	GT Bray	O ₃	Replacement of 2B Tech 202 with 2B Tech 211
12-086-6001	Homestead Fire Station	PM _{2.5}	A shutdown of SLAMS Manual 2025i. EXPECTED Q4 2021 Replacement of TEOM Continuous with T640 Continuous FEM monitor. EXPECTED Q4 2021
12-086-6002	Wittkop Park	PM _{2.5}	SU EXPECTED 12/2021
12-095-2002	Winter Park	CO, SO ₂ , NO ₂ , Ozone, PM10, PM2.5	Relocation Expected 10/2021
12-095-0011	Second near road	NO ₂ , CO	Orange County has requested a one year extension due to staffing changes and delays in the project. The original workplan approval was for the site to be running July 2021, the amended workplan requests a one year extension to be operational by July 2022.
12-099-2005	Delray Beach	PM _{2.5} , PM ₁₀	Replacement of MET One Bam 1020 with SLAMS T640X. Replacement of Manual Thermo 2025i with T640X Continuous FEM monitor. SU 4/2021
12-099-0008	Belle Glade	PM _{2.5}	Replacement of PM _{2.5} Met One BAM 1020 with Teledyne T640. SU EXPECTED 07/2021

3.1 SITE SHUT-DOWNS, SET-UPS AND RELOCATIONS

A. Site Shut-downs

Duval County – Cedar Bay: AQS Site # 12-031-0081

DEP is requesting approval to remove the SO₂ monitoring site located at Cedar Bay in Duval County as of March 29, 2021. This single pollutant monitoring site meets several scenarios defined in EPA's Network Assessment Guidance and 40 CFR 58.14(c), where the state or local agency can confidently request approval for the shutdown of a SLAMS monitor. These include:

- The monitor showed attainment during the last five years;
- The probability is less than 10% that this monitor will exceed 80% of the applicable NAAQS during the next three years based on the concentrations, trends, and variability observed in the past;
- The monitor is not specifically required by an attainment plan or maintenance plan, as it is an attainment area that is expected to remain in attainment; and
- The monitor has not measured violations of the SO₂ NAAQS in the last five years.

The removal of this monitor will allow more flexibility of resources and for greater emphasis to be placed on other criteria pollutants. A summary of the evaluation DEP performed for this monitor using EPA's Ambient Air Monitoring Network Assessment Guidance (AAMNAG) document is provided below in Table 3.2.

Table 3.2 Site and Monitor Evaluation Summaries for Discontinuation

AQS Site #	Site Name	Type	Pollutant	Showed Attainment 2015-2020	Probability <10% Monitor Will Exceed 80% of NAAQS	Monitor Specifically Required by Attainment or Maintenance Plan	Last Monitor in Nonattainment or Maintenance Area	CFR Required	Modification	Comments
12-031-0081	Cedar Bay	SLAMS	SO ₂	Yes	Yes	No	No	No	CLOSE	See calculations in Table 3.3

Section 4.1 of the AAMNAG states that a monitor can be removed (after Regional Administrator approval) if it is currently in attainment with the applicable NAAQS standard and if the following four tests can be met:

1. The PM_{2.5}, ozone, CO, PM₁₀, SO₂, lead, or NO₂ monitor showed attainment during the previous five years.
2. The probability is less than 10% that the monitor will exceed 80% of the applicable NAAQS during the next three years based on the concentrations, trends, and variability observed in the past. This can be done using the following equation:

$$\bar{X} + \frac{t*s}{\sqrt{n}} < 0.8 * \text{NAAQS}$$

\bar{X} is the average design value for the last 5 years

t is the student's t value for $n-1$ degrees of freedom at the 90% confidence level

s is the standard deviation of the design values

n is the number of records (i.e., number of design values)

NAAQS is the standard of interest.

3. The monitor is not specifically required by an attainment plan or maintenance plan.
4. The monitor is not the last monitor in a nonattainment area or maintenance area that contains a contingency measure triggered by an air quality concentration in the latest attainment or maintenance plan adopted by the state and approved by EPA.

All monitors listed in Table 3.2 passed these tests and the probability test results are listed in Table 3.3 below.

Table 3.3 40 CFR Part 58.14(c) and Ambient Air Monitoring Network Assessment Guidance Calculations

Site	Site Name	Pollutant	Averaging Period	Design Value					\bar{X}	s	t	n	NAAQS	80% of NAAQS	90% Confidence Interval	Pass
				2016	2017	2018	2019	2020								
12-031-0081	Cedar Bay	SO2	24-hr	20	12	11	10	9	12	3.4	2.13	5	75	60	15.23	Yes

Miami-Dade County – Homestead Fire Station Site

DEP was granted EPA approval October 2019 to relocate the Homestead Fire Station Site (AQS Site #: 12-086-6001) in Miami-Dade County due to structural integrity issues with the building. The Homestead Fire Station staff have also vacated the property to a more structurally sound facility. The new site, Wittkop Park, will be located approximately 850 meters northwest of the original site on the Homestead Public Services property and will be assigned a new AQS Site identification number (AQS Site # 12-086-6002) due to the change in address. Site review information for Homestead Fire Station is presented in Table 3.4 below with Wittkop Park information located in Table 3.5 and any other pertinent site information is provided in Appendix A.

Table 3.4 Homestead Fire Station - AQS Site # 12-086-6001

	Homestead Fire Station Site
AQS Site #	12-086-6001
City (CBSA)	Miami-Fort Lauderdale-West Palm Beach, FL
Site Name	Homestead Fire Station
Statement of Purpose	Needed by Regulation
Site Review Date	11/04/2020
County	Miami-Dade
Location Latitude	25.471931 N
Location Longitude	-80.482780 W
Address	325 NW 2 nd Street, Homestead, FL 33030
Objective	Population Exposure
Pollutants Monitored	PM2.5
Sampling and Analysis Method	PM _{2.5} : Thermo 2025i, Gravimetric Analysis and Continuous PM _{2.5} : TEOM 1400, Gravimetric Analysis
Spatial Scale	Neighborhood Scale
Operating Schedule	PM _{2.5} : 1-in-3-day and Continuous PM _{2.5} : Continuous
Network Type	SLAMS; PM _{2.5} Manual and Continuous
Distance from Inlet to nearest:	Tree drip line: Manual 25.0 m, Continuous 28.0 m Wall: 5.0 m Road: 228 m
Access	Unlimited
Owner of Land	Miami-Dade County
Inlet Height	PM _{2.5} Manual 7.06 m, Continuous 7.8 m
Comments	Relocation expected December 2021

B. Site Relocations

Miami-Dade County – Wittkop Park Site AQS # 12-086-6002

DEP was granted EPA approval October 2019 to relocate the Homestead Fire Station Site (AQS Site #: 12-086-6001) in Miami-Dade County due to structural integrity issues with the building. The new site, Wittkop Park, will be located approximately 850 meters northwest of the original site and will be assigned a new AQS Site identification number (AQS Site # 12-086-6002) due to the change in address. Florida Department of Environmental Protection is requesting to link these two sites. Miami is discontinuing the manual sampler and the TEOM 1400 from Homestead Fire Station and will start operation of their new Teledyne T640 at Wittkop Park. Site review information for Wittkop Park is presented in Table 3.5 below and any other pertinent site information is provided in Appendix A.

Table 3.5 Wittkop Park - AQS Site # 12-086-6002

	Wittkop Park
AQS Site #	12-086-6002
City (CBSA)	Miami
Site Name	Wittkop Park
Statement of Purpose	Needed by Regulation
Site Review Date	12/2/2020
County	Miami-Dade
Location Latitude	28.478249 N
Location Longitude	-80.483754 W
Address	505 NW 9 th Street, Homestead, FL 33030
Objective	Population Exposure
Pollutants Monitored	PM _{2.5}
Sampling and Analysis Method	PM _{2.5} : Teledyne T640 Continuous FEM , Broadband Spectroscopy
Spatial Scale	Neighborhood
Operating Schedule	Continuous PM _{2.5} :
Network Type	SLAMS
Distance from Inlet to nearest:	Estimated Drip line: 13.6 meters Wall: 16.8 meters Road: 14 meters
Access	Unlimited
Owner of Land	City of Homestead
Inlet Height	PM _{2.5} : Estimate 2.8 meters
Comments	The estimated coordinates of the new shelter are: 28.478249 N and -80.483754 W. Site relocation expected by October 2021.

Orange County – Winter Park

DEP is requesting approval to relocate the Winter Park (AQS Site #: 12-095-2002) in Orange County due to park construction. The shelter will be relocated on the same property, approximately 91 meters SW of its current location and will remain representative of the same air mass. Site Review information is presented in Table 3.6 and any other pertinent site information is provided in Appendix A.

Table 3.6 Winter Park - AQS Site # 12-099-2002

	Winter Park Site
AQS Site #	12-095-2002
City (CBSA)	Orlando-Kissimmee-Sanford, FL
Site Name	Winter Park
Statement of Purpose	Needed by Regulation
Site Review Date	2/9/2021
County	Orange
Location Latitude	28.596447 N
Location Longitude	-82.362429 W
Address	213 S. Denning Ave, Winter Park, FL 32789
Objective	Population Exposure (CO, NO2, PM10, PM2.5); High Concentration (SO2, O3)
Pollutants Monitored	CO, SO ₂ , NO ₂ , Ozone, PM ₁₀ , PM2.5,
Sampling and Analysis Method	CO: Thermo 48i. SO2: Thermo 43i. NO2: Thermo 42i. Ozone: Thermo 49i, UV Photometry; PM2.5: Thermo 5014i, Beta Attenuation; PM10: Thermo 5014i.
Spatial Scale	Neighborhood Scale (CO, O3, SO2, PM10, PM2.5); Urban (NO2)
Operating Schedule	Continuous
Network Type	SLAMS; SO₂, NO₂, O₃, PM₁₀, PM2.5; SPM; CO
Distance from Inlet to nearest:	Estimated Tree drip line: 11.8 m Wall: N/A Road: 121 m
Access	Unlimited
Owner of Land	City of Winter Park
Inlet Height	Continuous Gaseous 5.0 m; Particulates 5.2 m
Comments	Relocation on the same property 91 m SW of the current site.

4.0 FLORIDA'S AMBIENT AIR MONITORING NETWORK 2019

The Ambient Air Monitoring Section in Florida is responsible for measuring levels of regulated pollutants in the ambient air by maintaining a network of 90 monitoring stations across the state and measuring the concentration of pollutants such as ozone, lead, particles (dust), nitrogen oxides, sulfur dioxide, and carbon monoxide. These monitoring services are provided following EPA regulatory requirements. The criteria pollutant monitoring system is designed to make measurements to assess compliance with the national ambient air quality standards (NAAQS) as set by the EPA. The NAAQS defines air pollutant concentration levels judged necessary to protect public health and welfare. This section provides details of each pollutant network within Florida's ambient air monitoring network if all requests in this plan are granted.

4.1 OZONE NETWORK

Florida's PQAO operates an extensive ozone network covering the state from large urban areas to smaller rural areas totaling 56 monitoring sites. This network enables the state of Florida to learn how ozone is transported to and within the state, to identify the parts of the state with peak ozone concentrations, and to determine where ozone concentrations do and do not exceed the NAAQS. Table 4.1 lists all ozone monitoring stations within the state and their 2018-2020 design values.

Table 4.1 Florida's Ozone Network

AQS Site #	Site Name	Pollutant	2018-2020 Design Values
12-001-3012	Paynes Prairie Farm	Ozone	60
12-003-0002	Osceola National Forest - Olustee Ranger Station	Ozone	58
12-005-0006	St. Andrews State Park	Ozone	60
12-009-0007	Melbourne	Ozone	Not Available – Data Completeness
12-009-4001	Cocoa Beach	Ozone	60
12-011-0033	Vista View Park	Ozone	62
12-011-0034	Daniela Banu (NCore Site)	Ozone	59
12-011-2003	Pompano Highland Fire House	Ozone	59
12-011-8002	Dr. Von Mizell-Eula Johnson State Park	Ozone	60
12-021-0004	Laurel Oak Elementary	Ozone	59
12-023-0002	Lake City - Veterans Domicile	Ozone	Not Available – Data Completeness
12-031-0077	Sheffield Elementary	Ozone	59
12-031-0100	Mayo Clinic	Ozone	59
12-031-0106	Cisco Drive	Ozone	60
12-033-0004	Ellyson Industrial Park	Ozone	61
12-033-0018	Pensacola NAS	Ozone	62
12-035-0004	Flagler	Ozone	Not Available – Data Completeness
12-055-0003	Archbold Biological Station	Ozone	Not Available – Data Completeness
12-057-0081	E.G. Simmons Park	Ozone	67
12-057-1035	Davis Island (Coast Guard Station)	Ozone	59
12-057-1065	USMC Reserve Center	Ozone	67
12-057-3002	Sydney (NCore Site)	Ozone	64
12-059-0004	Bonifay Tri-County Airport	Ozone	58
12-069-0002	Clermont	Ozone	64
12-071-2002	Rotary Park	Ozone	62
12-071-3002	Bay Oaks Park	Ozone	60
12-073-0012	Tallahassee Community College	Ozone	59
12-081-3002	Port Manatee	Ozone	63

12-081-4012	GT Bray Park	Ozone	64
12-081-4013	39th Street Park	Ozone	61
12-083-0003	Ocala - YMCA	Ozone	61
12-083-0004	Marion County Sheriff	Ozone	59
12-085-0007	Stuart	Ozone	60
12-086-0027	Rosenstiel (University of Miami)	Ozone	58
12-086-0029	Perdue	Ozone	61
12-091-0002	Fort Walton Beach	Ozone	60
12-095-0010	Skyview	Ozone	Not Available – Site Opened 3/2020
12-095-2002	Lake Isle Estates - Winter Park	Ozone	63
12-097-2002	Osceola Co. Fire Station - Four Corners	Ozone	66
12-099-0021	Lantana Preserve	Ozone	59
12-099-0022	Lamstein Lane	Ozone	Not Available - Site opened 1/2019
12-101-0005	San Antonio	Ozone	60
12-101-2001	Holiday	Ozone	64
12-103-0004	St. Petersburg College	Ozone	66
12-103-0018	Azalea Park	Ozone	63
12-103-5002	John Chesnut Sr. Park - East Lake	Ozone	61
12-105-6005	Sikes Elementary School	Ozone	64
12-105-6006	Baptist Children's Home	Ozone	65
12-111-0013	Savannas	Ozone	59
12-113-0015	Woodlawn Beach Middle School	Ozone	62
12-115-1005	Lido Park	Ozone	60
12-115-1006	Paw Park	Ozone	63
12-115-2002	Jackson Road	Ozone	60
12-117-1002	Seminole Community College	Ozone	62
12-127-5002	Daytona - Blind Services	Ozone	59
12-129-0001	St. Marks Wildlife Refuge (NCore Site)	Ozone	57

4.2 PM_{2.5} NETWORK

The Federal Reference Method and Federal Equivalent Method Network

Florida's PQAO currently operates 9 federal reference methods (FRM) and 27 federal equivalent method (FEM) monitors, for a total 36 monitors of which there are 27 primary monitors and 8 collocated. There is an approved waiver for the FEM Met One BAM 1020 instruments operating in Palm Beach County to remain, non-regulatory monitors since they do not meet the required FEM statistics in 40 CFR Part 53(C). Palm Beach County is expected to replace the Met One BAM 1020 by June 2021 with an approved FEM monitor, the Teledyne T640. The 26 other FEM monitors have been approved by the EPA and can be used to determine compliance with the NAAQS. This network is sufficient to protect the health and welfare of Florida's residents and environment. It also provides information on how fine particles are transported to and within the state, to identify the parts of the state with the highest concentrations of fine particles, and to determine where fine particle concentrations do and do not exceed the NAAQS. All of Florida's PM_{2.5} monitoring sites, with valid design values for 2018-2020, are less than 80 percent of the annual standard (9.6 µg/m³) as detailed in Table 4.2.

Table 4.2 Florida's PM_{2.5} Network

AQS Site #	Site Name	Pollutant	Method: FRM/FEM	Operating Schedule	2018-2020 Design Values	Comments
12-001-3012	Paynes Prairie Farm	PM _{2.5}	FEM	Continuous	6.9	
12-009-0007	Melbourne	PM _{2.5}	FEM	Continuous	6.5	
12-011-0034	Daniela Banu (NCore Site)	PM _{2.5}	FRM	Manual	6.6	
		PM _{2.5}	FEM	Continuous		Collocated
12-011-0035	Fort Lauderdale Near Road	PM _{2.5}	FEM	Continuous	9.1	
12-011-2003	Pompano Highland Fire House	PM _{2.5}	FEM	Continuous	6.7	
12-011-5005	Coconut Creek	PM _{2.5}	FEM	Continuous	6.7	
12-031-0098	Mandarin Rd Site	PM _{2.5}	FRM	Every 3rd Day	7.1	
12-031-0099	Sunny Acres	PM _{2.5}	FRM	Every 3rd Day	6.8	
			FRM	Every 12th Day		Collocated monitor
12-031-0108	Pepsi Place (PP-PPL)	PM _{2.5}	FEM	Continuous	8.5	
12-033-0004	Ellyson Industrial Park	PM _{2.5}	FEM	Continuous	8.6	
12-057-0113	Munro Street	PM _{2.5}	FEM	Continuous	Not Available – Data Completeness	

12-057-3002	Sydney (NCore Site)	PM _{2.5}	FRM	Every 3 rd Day	7.8	
			FEM	Continuous		Collocated monitor
12-071-0005	Winkler Pump Station	PM _{2.5}	FEM	Continuous	7.4	
			FEM	Continuous		Collocated monitor
12-073-0012	Tallahassee Community College	PM _{2.5}	FRM	Every 3rd Day	7.5	
			FRM	Every 12th Day		Collocated monitor
12-086-0033	Palm Springs Fire Station	PM _{2.5}	FRM	Every 3rd Day	6.5	
12-086-1016	Miami Fire Station	PM _{2.5}	FEM	Continuous	7.9	
			FRM	Every 12th Day		Collocated monitor
12-086-6001	Homestead Fire Station	PM _{2.5}	FRM	Every 3rd Day	6.8	
			FEM	Continuous		Collocated
12-095-0009	I-4 Near Road	PM _{2.5}	FEM	Continuous	Not Available – Site has a temporary monitoring waiver	
12-095-2002	Lake Isle Estates - Winter Park	PM _{2.5}	FEM	Continuous	6.7	
12-099-0008	Belle Glade	PM _{2.5}	FEM	Continuous	Non- regulatory Monitor	
12-099-0022	Lamstein Lane	PM _{2.5}	FEM	Continuous	Not Available – Site opened 1/2019	
			FEM	Continuous		Collocated monitor
12-099-2005	Delray Beach	PM _{2.5}	FEM	Continuous	6.2	
12-103-0004	St. Petersburg College	PM _{2.5}	FEM	Continuous	Not Available – Monitor opened 3/2019	
12-103-0018	Azalea Park	PM _{2.5}	FEM	Continuous	7.6	
12-105-6006	Baptist Children's Home	PM _{2.5}	FEM	Continuous	7.8	
12-115-0013	Bee Ridge Park	PM _{2.5}	FEM	Continuous	7.1	
12-117-1002	Sanford	PM _{2.5}	FEM	Continuous	6.9	
			FRM	Every 12th Day		Collocated monitor
12-127-5002	Daytona - Blind Services	PM _{2.5}	FEM	Continuous	7.5	

4.3 NCORE NETWORK

The National Core (NCore) monitoring network is designed to be approximately 80 sites nationwide, with the intent to have a network made of largely population-oriented sites and some rural sites that take advantage of multi-pollutant monitoring. Details of the NCORE network are provided on EPA's website at <https://www.epa.gov/amtic/ncore-monitoring-network>. Table 4.3 provides information on Florida's NCORE sites.

Table 4.3 NCORE Sites in Florida

AQS Site #	Site Name	Parameter
12-129-0001	St. Marks National Wildlife Refuge	O ₃ , NO _y , CO, SO ₂ _TL, Continuous PM _{2.5}
12-011-0034	Daniela Banu	O ₃ , NO _y _TL, NO _z _TL, NO_TL, CO_TL, SO ₂ _TL, Continuous PM _{2.5} , PM _{10-2.5} , Low Volume PM ₁₀ , PM ₁₀ and PM _{2.5}
12-057-3002	Sydney	O ₃ , NO _y _TL, NO _z _TL, NO_TL, CO_TL, SO ₂ _TL, Continuous PM _{2.5} , PM _{10-2.5} , Low Volume PM ₁₀ , PM ₁₀ and PM _{2.5}

EPA only requires two NCORE monitoring sites for the State of Florida, but the PQAO currently operates three sites. EPA requested that DEP operate a rural NCORE site at the St. Marks National Wildlife Refuge to enhance the coverage for the southeastern United States. The St. Marks National Wildlife Refuge site (AQS Site #12-129-0001) takes advantage of the existing Interagency Monitoring of Protected Visual Environments (IMPROVE) and DEP monitoring for particulate matter and ozone, respectively.

Building on the Speciation Trends Network (STN), the two required NCORE sites are located in the largest Metropolitan Statistical Areas in the state - the Miami-Fort Lauderdale-Miami Beach area (more than 6 million) and Tampa-St. Petersburg-Clearwater area (more than 2 million). In the Miami-Fort Lauderdale-Miami Beach area, the NCORE site is Daniela Banu (AQS Site#12-011-0034), which is operated by Broward County. The site began operation in August 2015 and the meteorological instruments have been operational since January 2020.

In the Tampa-St. Petersburg-Clearwater area, the NCORE site is Sydney (AQS Site #12-057-3002), which is operated by Hillsborough County. This site was used as part of a large and intense nitrogen deposition study called the Bay Regional Atmospheric Chemistry Experiment (BRACE). It has also been monitoring trace SO₂, CO and total reactive nitrogen (NO_y) since 2004. Since the primary use of the NCORE sites is to obtain air quality trends analyses, Sydney's location in a more rural part of the county is ideal for tracking trends that reflect the increasing population.

4.4 PAMS NETWORK

The NCORE sites in Metropolitan Statistical Areas with populations over one million will be required to incorporate the Photochemical Assessment Monitoring Station (PAMS) program in accordance with 40 CFR part 58, Appendix D, section 5(a). The PAMS measurements include:

1. Hourly averaged speciated volatile organic compounds (VOCs);
2. Three eight-hour averaged carbonyl samples per day on a 1 in 3-day schedule, or hourly averaged formaldehyde;
3. Hourly averaged O₃;
4. Hourly averaged nitrogen oxide (NO), true nitrogen dioxide (NO₂), and total reactive nitrogen (NO_y);
5. Hourly averaged ambient temperature;
6. Hourly vector-averaged wind direction;
7. Hourly vector-averaged wind speed;
8. Hourly average atmospheric pressure;
9. Hourly averaged relative humidity;
10. Hourly precipitation;
11. Hourly averaged mixing-height;
12. Hourly averaged solar radiation; and
13. Hourly averaged ultraviolet radiation.

The Daniela Banu (AQS Site #12-011-0034) and Sydney (AQS Site #12-057-3002) NCORE sites located in Broward and Hillsborough counties, respectively, will be required to implement PAMS monitoring. The Broward and Hillsborough counties have created a separate Primary Quality Assurance Organization (PQAO) for the PAMS network, hereafter known as the Florida PAMS PQAO. The Florida PAMS PQAO will continue preparing to implement the program as funding and personnel resources allow with the goal of full implementation on or before June 1, 2021. The PAMS Network Plan for each county is provided below, these are new parameters at the existing sites utilized for the NCORE network.

PAMS Monitoring Implementation Network Plan – Broward County

PAMS Monitoring Site: Daniela Banu AQS Site # 12-011-0034 PAMS site utilizes the NCORE network at Daniela Banu.

POLLUTANT	OPERATING SCHEDULE	SAMPLER	MONITORING OBJECTIVE	SPATIAL SCALE
NMHC	Continuous, O3 season ONLY	CAS Auto- GC FID	POP EXP	NBH
Carbonyls	3 - 8 hour samples, 1-in-3, during national O3 season ONLY	ATEC 8000	POP EXP	NBH
NO	Continuous	Teledyne T500	POP EXP	NBH
NO2	Continuous	Teledyne T500	POP EXP	NBH
UV/Solar Radiation	Continuous	Kipp & Zonen SUV5-V & SMP6-V	POP EXP	NBH
Precipitation Gage	Continuous	RM Young 52202	POP EXP	NBH
Atmospheric Pressure Gauge	Continuous	RM Young 61302L	POP EXP	NBH
Mixing Height	Continuous, during national O3 season ONLY	Vaisala CL51 Celiometer	POP EXP	NBH

PAMS Monitoring Implementation Network Plan – Hillsborough County

PAMS Monitoring Site: Sydney AQS Site # 12-057-3002 PAMS site utilizes the NCORE network at Sydney.

POLLUTANT	OPERATING SCHEDULE	SAMPLER	MONITORING OBJECTIVE	SPATIAL SCALE
NMHC	Continuous, O3 season ONLY	CAS Auto- GC FID	POP EXP	NBH
Carbonyls	3 - 8 hour samples, 1-in-3, during national O3 season ONLY	ATEC 8000	POP EXP	NBH
NO	Continuous	Teledyne T500	POP EXP	NBH
UV/Solar Radiation	Continuous	Kipp & Zonen SUV5-V & SMP6-V	POP EXP	NBH
Precipitation Gage	Continuous	RM Young 52202	POP EXP	NBH
Atmospheric Pressure Gauge	Continuous	RM Young 61302L	POP EXP	NBH
Mixing Height	Continuous, during national O3 season ONLY	Vaisala CL51 Ceilometer	POP EXP	NBH

4.5 NATTS NETWORK

The National Air Toxics Trends Station (NATTS) Network was developed to fulfill the need for long-term Hazardous Air Pollutants (HAPs) monitoring data of consistent quality. Among the principle objectives are assessing trends and emission reduction program effectiveness, as well as assessing and verifying air quality models. The current NATTS network configuration includes 27 sites (20 urban, 7 rural) across the United States. There are typically more than 100 pollutants monitored at each NATTS, although only 19 are required. These include VOCs, carbonyls, PM₁₀ metals, hexavalent chromium and Polycyclic Aromatic Hydrocarbons (PAHs). Table 4.4 lists the NATTS sites in Hillsborough and Pinellas counties. These counties jointly administer funds for the NATTS program. The two NATTS sites in Florida are in the Tampa Bay area: one in Hillsborough County (Sydney: AQS Site #12-057-3002) and the other in Pinellas County (Skyview: AQS Site #12-103-0026). The NATTS/Air Toxics QAPP was approved in November 2019.

Table 4.4 NATTS Sites in Florida

AQS Site #	Site Name	County	Pollutants
12-103-0026	Skyview	Pinellas	VOCs, Carbonyls, PAHs and Metals
12-057-3002	Sydney (NCore Site)	Hillsborough	VOCs, Carbonyls and Metals

4.6 SO₂ MONITORING NETWORK

Florida's air monitoring network complies with current SO₂ monitoring requirements. Ambient monitoring is required for Core Based Statistical Areas (CBSAs) whose Population Weighted Emission Index (PWEI) is above 5,000. One SO₂ monitor is required for CBSAs when the PWEI is above 5,000 and two monitors are required when the PWEI is above 100,000, with a unit of million persons-ton per year. Additionally, one SO₂ monitor is required at each of the NCores sites. A summary of these requirements is provided in Table 4.5. The PWEI values listed were provided by EPA.

Table 4.5 SO₂ Monitoring Requirements

Core Based Statistical Areas	Counties	2019 Census Population	Total CBSA Emissions	PWEI 2017 NEI	SO ₂ Monitors Needed	SO ₂ Monitors Operating
Miami-Fort Lauderdale ² - Pompano Beach	Broward, Miami-Dade, Palm Beach	6,166,488	5,378.63	33,167.24	1	2
Tampa ² -St. Petersburg-Clearwater	Hernando, Hillsborough, Pasco, Pinellas	3,194,831	8,940.77	28,564.24	1	6
Orlando-Kissimmee-Sanford	Lake, Orange, Osceola, Seminole	2,608,147	4,826.09	12,587.14	1	1
Jacksonville ¹	Baker, Clay, Duval, Nassau, St. Johns	1,559,514	9,832.24	15,333.52	1	3
North Port-Sarasota-Bradenton	Manatee, Sarasota	836,995	816.43	683.35		1
Cape Coral-Fort Myers	Lee	770,577	361.05	278.22		
Lakeland-Winter Haven	Polk	724,777	15,598.24	11,305.24	1	1
Deltona-Daytona Beach-Ormond Beach	Volusia	668,365	195.15	130.43		
Palm Bay-Melbourne-Titusville	Brevard	601,942	350.87	211.20		
Pensacola-Ferry Pass-Brent	Escambia, Santa Rosa	502,629	2,476.04	1,244.53		1
Port St. Lucie	Martin, St. Lucie	489,297	650.25	318.16		
Palatka	Putnam	74,521	5,895.17	439.31		1

Tallahassee ²	Gadsden, Jefferson, Leon, Wakulla	387,227	1,123.27	434.96		1
Homosassa Springs	Citrus	149,657	12,824.17	1,919.23		1
N/A	Hamilton	14,326	N/A	N/A		1
Total					5	19

¹ SO₂ at Cedar Bay shutdown 3/29/2021

² CBSA operates a NCORE site

Table 4.6 Florida's SO₂ Network

AQS Site #	Site Name	Pollutant	Monitoring Purpose
12-011-0034	Daniela Banu (NCore Site)	SO ₂	Population
12-017-0006	Crystal River Preserve	SO ₂	Source
12-031-0032	Kooker Park	SO ₂	Data Trends
12-031-0081	Cedar Bay STP ¹	SO ₂	Source
12-033-0004	Ellyson Industrial Park	SO ₂	Population
12-047-0015	White Springs	SO ₂	Source
12-057-0112	Apollo Beach	SO ₂	Source
12-057-0109	East Bay	SO ₂	Source
12-057-1035	Davis Island (Coast Guard Station)	SO ₂	Population
12-057-3002	Sydney (NCore Site)	SO ₂	Population
12-081-0028	Port Manatee DEP	SO ₂	Source
12-086-0019	Pennsuco	SO ₂	Population
12-089-0005	Fernandina Beach Waste Water Treatment Plant	SO ₂	Regulatory
12-095-2002	Lake Isle Estates - Winter Park	SO ₂	Regulatory
12-103-0023	Derby Lane	SO ₂	Population
12-103-5003	Oakwood	SO ₂	Source
12-105-6005	Sikes Elementary School	SO ₂	Regulatory
12-107-1008	Palatka Barge Port	SO ₂	Source
12-129-0001	St. Marks Wildlife Refuge (NCore Site)	SO ₂	Background

¹SO₂ at Cedar Bay shutdown 3/29/2021

4.7 NO₂ MONITORING NETWORK

There are two phases for the implementation of NO₂ Near-road monitoring:

- Phase I: CBSAs with a population over 1 million are required to have at least one NO₂ near-road monitor
- Phase II: CBSAs with a population over 2.5 million or more are required to operate two NO₂ near-road monitors.

Phase I and II NO₂ Near-road monitoring also require community-wide monitoring for areas with a population over 1 million and NO₂ monitoring of vulnerable and susceptible populations.

In Florida, the NO₂ near-road monitoring areas are Tampa, Fort Lauderdale, Jacksonville and Orlando. All Phase I NO₂ near-road sites within these areas have been established. However, the Phase I near-road NO₂ site (I-4 Near Road: AQS Site #: 12-095-0009) in Orange County received a temporary monitoring waiver from EPA Region 4 in July 2017, due to ongoing I-4 construction which resulted in environmental conditions not representative of the ambient air.

The 2018 census estimates indicated that the population for the Orlando-Kissimmee CBSA is now above 2.5 million and as a result will require a second NO₂ near-road site. Florida DEP, Orange County and EPA Region 4 are working collaboratively on the implementation of this site. The goal is to have the site location selected by July 1, 2021 and the site operational within one year thereafter. A Network Plan Addendum will be submitted to EPA Region 4 for review and approval once the details have been finalized.

All other Phase II NO₂ near-road sites located in the Tampa-Saint Petersburg-Clearwater (Sawgrass Lake Park: AQS Site #12-103-0027) and Miami-Fort Lauderdale-Pompano Beach (Perimeter Road: AQS Site #12-086-0035) CBSAs are currently established and operational.

A summary of the NO₂ monitoring requirements is provided in Table 4.7 and the designated community-wide and vulnerable and susceptible monitors for the state are provided in Table 4.8.

Table 4.7 NO₂ Monitoring Required by 2010 NAAQS

CBSAs with Population over 1,000,000	2018 Census Population	AADT ≥250,000	Required Near-road Monitors	Required Community-wide Monitor	Vulnerable and Susceptible	Total
Miami-Fort Lauderdale-Pompano Beach	6,198,782	✓	2 ¹	1	1	4
Tampa-St. Petersburg-Clearwater	3,142,663	N/A	2 ¹	1	N/A	3
Orlando-Kissimmee	2,572,962	N/A	2 ¹	1	N/A	3
Jacksonville	1,534,701	N/A	1	1	N/A	2
Total						12

¹ Population greater than 2.5 million requires two near-road sites.

Community-wide NO₂ Monitoring

Community-wide NO₂ monitoring sites are required in each CBSA with a population of 1 million or more. In Florida, there are four CBSAs that meet this criterion: Miami-Fort Lauderdale-Miami Beach, Tampa-St. Petersburg-Clearwater, Orlando-Kissimmee and Jacksonville. The NO₂ monitors that have been designated as community-wide monitors are listed in Table 4.8 below.

Vulnerable and Susceptible Monitoring

The 2010 NO₂ NAAQS revision included monitoring requirements for vulnerable and susceptible populations. Vulnerable populations are those exposed to higher concentrations of NO₂, such as individuals living and working near high traffic volume highways, and this exposure will be monitored with the near-road network. Susceptible populations are those affected by lower levels of NO₂ or that experience a larger health impact than the general population to a given level of exposure. Per EPA's Integrated Science Assessment for Oxides of Nitrogen-Health Criteria, factors that can confer susceptibility include pre-existing diseases (e.g., asthma).

Florida participates in the National Environmental Public Health Tracking Network supported by the U.S. Centers for Disease Control. This program examines health and environmental data to help federal, state and local agencies plan, apply and develop environmental public health actions. Higher crude rate of asthma hospitalizations has been used as an indicator of vulnerable and susceptible communities in Florida. Miami-Dade County's NO₂ site, located at the University of Miami, Rosenstiel (AQS Site #12-086-0027), has been designated as a vulnerable and susceptible monitoring site for NO₂. Figure 4.1 provides the most recent year of Florida's crude rate of asthma hospitalization by county for which data are available. A link to the full list of the NO₂ monitors identified by the Regional Administrators can be found on EPA's website at <https://www.epa.gov/amtic/no2-monitoring-near-road-monitoring>.

Figure 4.1 2019 Crude Rate of Asthma hospitalizations, Rate Per 100,000 Population

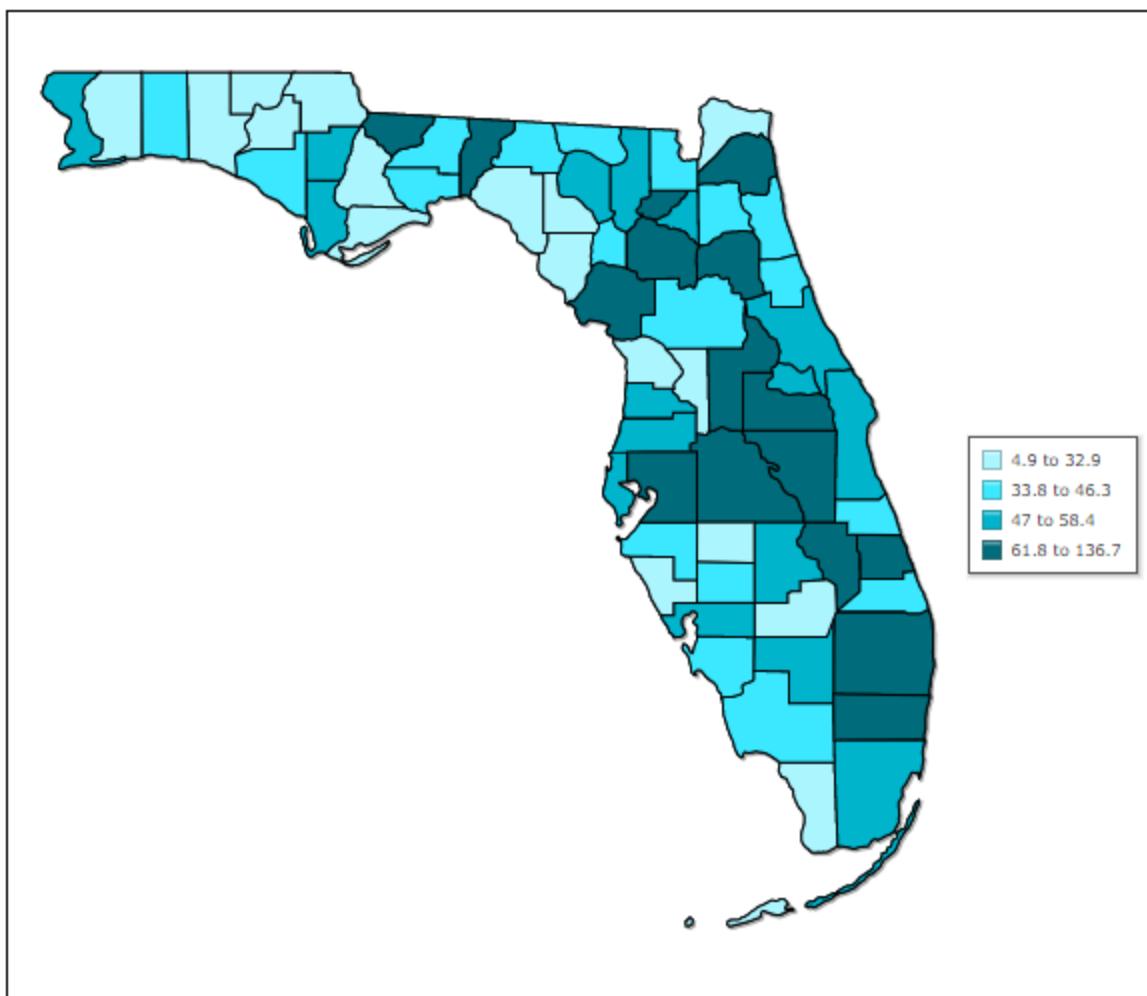


Table 4.8 Florida's NO₂ Near-road Network and Monitor Designations

CBSAs with Population over 500,000	AQS Site #	Site Name	Designation
Miami-Fort Lauderdale-Pompano Beach	12-011-0035	Fort Lauderdale Near-road	NO ₂ Near-road
	12-011-8002	Dr. Von Mizell-Eula Johnson State Park	NO ₂ Community-wide Monitor
	12-086-0027	Rosenstiel (University of Miami)	NO ₂ Vulnerable and Susceptible monitor
	12-086-0035	Perimeter Road Near-road	NO ₂ Near-road
	12-086-4002	Lab Annex	NO ₂ Network
	12-099-0021	Lantana Preserve	NO ₂ Network
Tampa-St. Petersburg-Clearwater	12-057-0113	Munro Street Near-road	NO ₂ Near-road
	12-057-1065	USMC Reserve Center	NO ₂ Network
	12-103-0018	Azalea Park	NO ₂ Community-wide Monitor
	12-103-0027	Sawgrass Lake Park Near-road	NO ₂ Near-road
Orlando-Kissimmee	12-095-0009	I-4 Near-road ¹	NO ₂ Near-road
	12-095-2002	Lake Isle Estates – Winter Park	NO ₂ Community-wide Monitor
Jacksonville	12-031-0032	Kooker Park	NO ₂ Community-wide Monitor
	12-031-0108	Pepsi Place Near-road	NO ₂ Near-road

¹ Orlando-Kissimmee near-road site has an approved temporary monitoring waiver as of 7/1/2017.

The approval letter for discontinuance, along with a detailed description and images of construction, for the Orlando-Kissimmee I-4 Near Road site (AQS Site: 12-095-0009) are found in Appendix A .

4.8 CO MONITORING NETWORK

Florida's carbon monoxide (CO) network covers large urban areas to smaller rural areas, totaling 9 monitoring sites. This network enables the state of Florida to monitor the consistent decrease in CO emissions within the state and to identify the parts of the state with peak CO concentrations. Table 4.9 lists all CO monitoring stations within the state and any exceedances for calendar years 2018 to 2020.

Table 4.9 Florida's CO Network

AQS Site #	Site Name	Pollutant	Exceedances for 2018-2020	Comments
12-011-0034	Daniela Banu (NCore Site)	CO	0	
12-011-0035	Fort Lauderdale Near Road	CO	0	Supports Near-road NO ₂ Monitoring
12-031-0108	Pepsi Place	CO	0	Supports Near-road NO ₂ Monitoring
12-057-0113	Munro Street	CO	0	Supports Near-road NO ₂ Monitoring
12-057-3002	Sydney (NCore Site)	CO	0	
12-086-4002	Lab Annex	CO	0	
12-095-2002	Lake Isle Estates - Winter Park	CO	0	
12-103-0027	Sawgrass Lake Park	CO	0	Supports Near-road NO ₂ Monitoring
12-129-0001	St. Marks Wildlife Refuge (NCore Site)	CO	0	

4.9 PM₁₀ MONITORING NETWORK

The Federal Reference Method and Federal Equivalent Method Network

Florida's PQAO currently operates 20 federal equivalent method (FEM) monitors. This network is sufficient to protect the health and welfare of Florida's residents and environment. It also provides information on how PM₁₀ particles are transported to and within the state, to identify the parts of the state with the highest concentrations, and to determine where PM₁₀ concentrations do and do not exceed the NAAQS. There is an approved siting criteria waiver for the source-oriented Woodlawn site in Pinellas County (AQS Site # 12-103-0012). Information for re-evaluation of this waiver is provided in section 5.0 of this plan. All of Florida's PM₁₀ monitoring sites meet the NAAQS for calendar years 2018 to 2020, as detailed in Table 4.10.

Table 4.10 Florida's PM₁₀ Network

AQS Site #	Site Name	Pollutant	Method: FRM/FEM	Operating Schedule	Exceedances for 2018- 2020	Comments
12-009-0007	Melbourne	PM ₁₀	FEM	Continuous	0	
12-011-0034	Daniela Banu (NCore Site)	PM ₁₀	FEM	Continuous	0	
12-011-5005	Coconut Creek	PM ₁₀	FEM	Continuous	0	
12-031-0032	Kooker Park	PM ₁₀	FEM	Continuous	0	
12-031-0098	Mandarin Rd Site	PM ₁₀	FEM	Continuous	0	
12-033-0004	Ellyson Industrial Park	PM ₁₀	FEM	Continuous	0	
12-057-0083	Gardinier Park	PM ₁₀	FEM	Continuous	0	
12-057-1035	Davis Island (Coast Guard Station)	PM ₁₀	FEM	Continuous	0	
12-071-0005	Winkler Pump Station	PM ₁₀	FEM	Continuous	0	
12-086-1016	Miami Fire Station	PM ₁₀	FEM	Continuous	0	
12-091-0002	Fort Walton Beach	PM ₁₀	FEM	Continuous	0	
12-095-2002	Lake Isle Estates - Winter Park	PM ₁₀	FEM	Continuous	0	
12-099-2005	Delray Beach	PM ₁₀	FEM	Continuous	0	
12-103-0012	Woodlawn	PM ₁₀	FEM	Continuous	0	
12-103-0018	Azalea Park	PM ₁₀	FEM	Continuous		
12-103-3004	County Motorpool	PM ₁₀	FEM	Continuous	0	
12-105-6006	Baptist Children's Home	PM ₁₀	FEM	Continuous	0	
12-107-1008	Palatka Barge Port	PM ₁₀	FEM	Continuous	0	

12-115-1006	Paw Park	PM ₁₀	FEM	Continuous	0	
12-117-1002	Seminole Community College	PM ₁₀	FEM	Continuous	0	
12-127-5002	Daytona - Blind Services	PM ₁₀	FEM	Continuous	0	

4.10 LEAD MONITORING NETWORK

Florida's PQAO currently operates 3 lead (Pb) source monitors. This network is sufficient to protect the health and welfare of Florida's residents and environment. It also provides information on how Pb particles are transported to and within the state due to the known sources and to determine where Pb source concentrations do and do not exceed the NAAQS. All of Florida's Pb monitoring sites and their 2018 to 2020 design values are detailed in Table 4.11 below.

Table 4.11 Florida's Lead Source Monitoring Network

AQS Site #	Site Name	2018-2020 Design Values
12-057-0100	Kenly	0.01
12-057-1066	Gulf Coast Lead	0.11
12-057-1073	Patent Scaffolding	0.06

5.0 MONITORING WAIVERS

A. SITING CRITERIA

Per 40 CFR 58, Appendix E, Section 10: Waiver Provisions, EPA will consider a written request from the State agency to waive one or more siting criteria for some monitoring sites if the State can adequately demonstrate the need (purpose) for monitoring at that location. For existing sites, a waiver may be granted if either of the criteria in sections 10.1.1 and 10.1.2 is met:

- The site can be demonstrated to be as representative of the monitoring area as it would be if the siting criteria were being met.
- The monitor or probe cannot reasonably be located to meet the siting criteria because of physical constraints (e.g., inability to locate the required type of site the necessary distance from roadways or obstructions).

In this section, DEP demonstrates that the siting waiver requests below meet the criteria of 10.1.1 or 10.1.2, and request approval from the EPA's Regional Administrator.

- *Miami-Dade County – Rosenstiel (University of Miami)*

DEP is requesting a waiver from the probe height siting requirements, per the criteria stated in section 10.1.2, for the NO₂ and O₃ sampler in Miami-Dade County at the Rosenstiel site, AQS Site # 12-086-0027. A site review conducted on November 30, 2020, found that the siting requirements in 40 CFR Part 58 Appendix E, Table E-4 could not be met. The site has historic data dating back to 1984 and site reviews consistently shows the probe height to be above 15 meters as far back as 2006. The most recent site review information is provided in Table 5.1.

The site is located on Virginia Key, a barrier island in Miami-Dade County, on the roof of the University of Miami's Rosenstiel School of Marine and Atmospheric Sciences building. The probe height is 16.3 meters from the ground to the probe inlet, and there is unrestricted airflow 270° around the sampler. Moving the probe inlet 1.3 meters down would mean that it would be impossible to meet the 2 to 15 meters above ground level. Miami-Dade County would prefer to continue the operation of the site to meet local interests and to continue to provide educational and research benefits. In addition, relocation of this site on the barrier island is not feasible given its sensitive location, as Virginia Key is mostly a protected public park, with highly restrictive coastal building codes along this storm prone area.

Data collected pre-and post-discovery of siting issues correlate well and show negligible variability for the NO₂ and O₃ concentrations. Additionally, a data comparison of NO₂ and O₃ at Rosenstiel (12-086-0027) to O₃ at Perdue (12-086-0029) and NO₂ at Lab Annex (12-086-4002) demonstrates levels are consistently below the NAAQS for NO₂ and O₃ concentrations from 2011-2019 (see Figures 5.5 through 5.8 below).

Figure 5.1 2020 Site Review of Rosenstiel (University of Miami) – AQS Site #12-086-0027

AQS Site #	12-086-0027
City (CBSA)	Miami-Fort Lauderdale-Pompano Beach, FL
Site Name	Rosenstiel (University of Miami)
Statement of Purpose	NO ₂ ; Vulnerable and Susceptible Monitoring; O ₃ ; Needed by regulation
Site Review Date	11/30/2020
County	Miami-Dade County
Location Longitude	-80.161750
Location Latitude	25.732878
Address	4600 Rickenbacker Causeway, Miami, FL 33149
Objective	Population Exposure
Pollutants Monitored	NO ₂ , Ozone
Sampling and Analysis Method	NO ₂ (Teledyne T200), Ozone (Thermo 49i)
Spatial Scale	NBH
Operating Schedule	Continuous
Network Type	SLAMS
Distance from Inlet to nearest:	Wall/Inlet: Building 10.0 meters Tree Dripline: Palm Tree 29.0 meters Road: 60.0 meters
Access	Unlimited
Inlet Height	16.3 meters
Comments	The Ozone & NO ₂ inlets are above the 15 m limit. The height from the ground to the probe inlet is 16.3 meters.

Figure 5.2 South facing in



Figure 5.3 From Ground East facing in



Figure 5.4 Aerial of Rosenstiel



Figure 5.5 Annual Average of Ozone from Rosenstiel 086-0027 and Purdue 086-0029

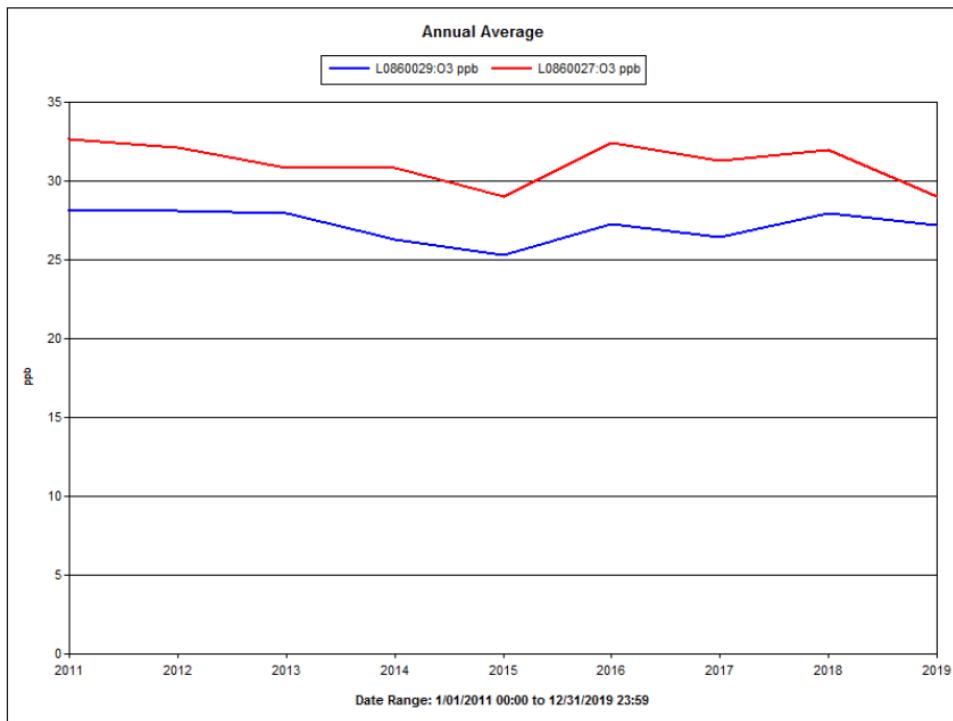


Figure 5.6 Daily Max 8-Hour Rolling Average of Ozone from Rosenstiel 086-0027 and Purdue 086-0029

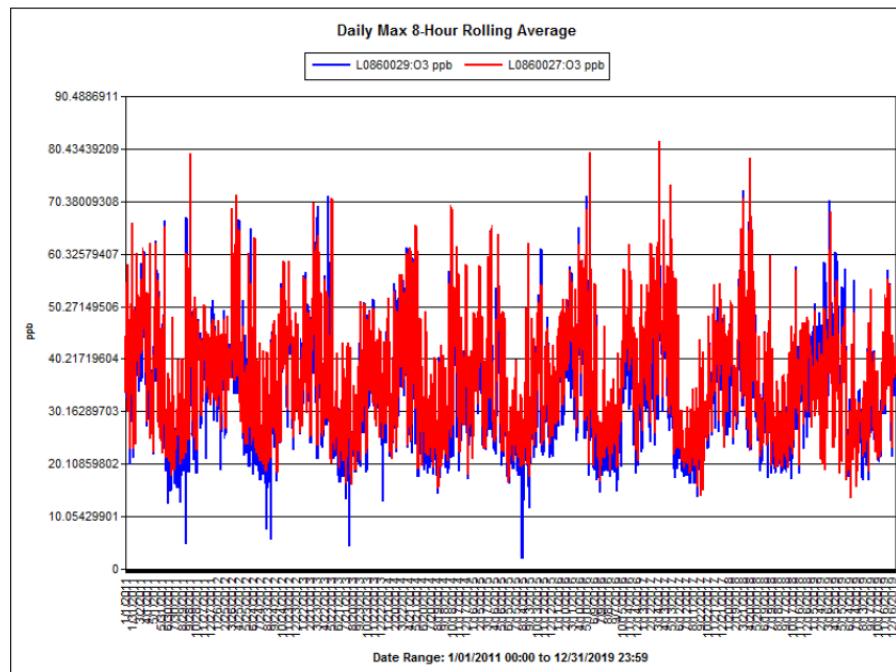


Figure 5.7 Annual Average of Nitrogen Dioxide from Rosenstiel 086-0027 and Lab Annex 086-4002


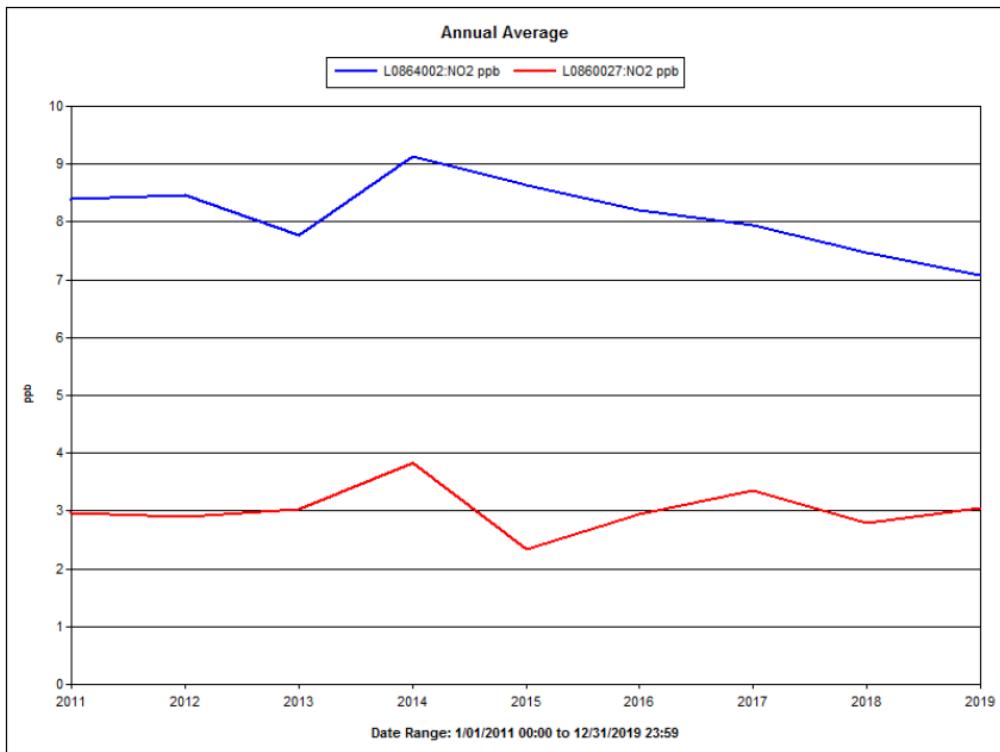


Figure 5.8 Daily Max 1-Hour Average of Nitrogen Dioxide from Rosenstiel 086-0027 and Lab Annex 086-4002

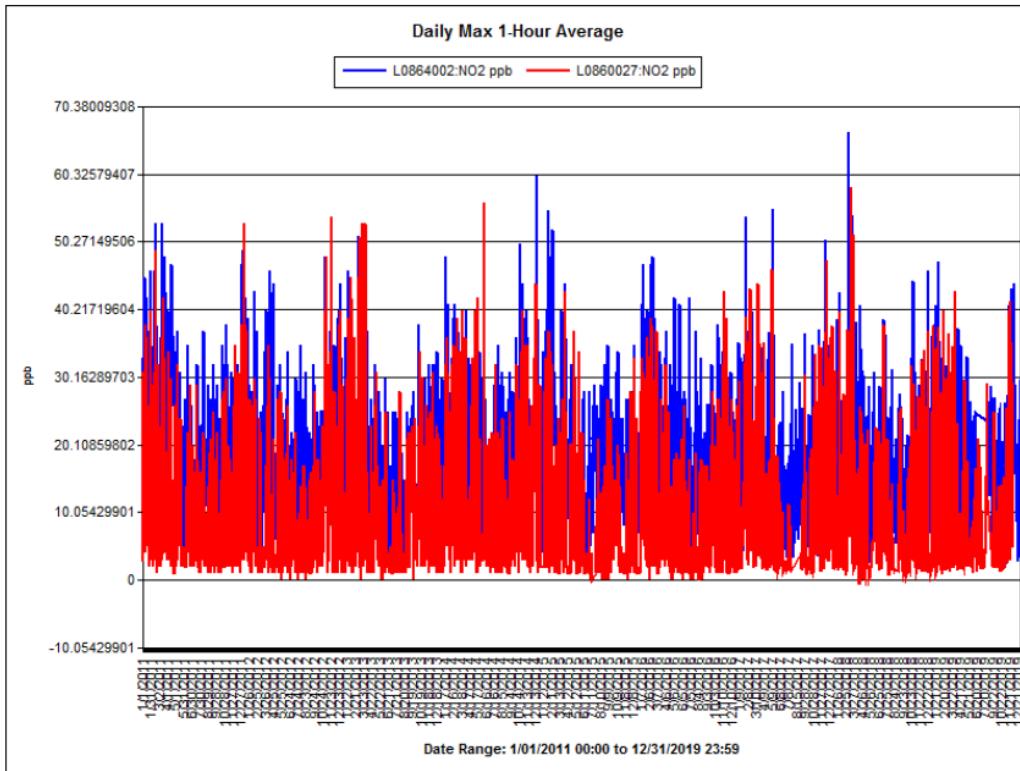

Pinellas County - Woodlawn

DEP is requesting the continuance of an approved waiver from the dripline siting requirements for the PM₁₀ monitor in Pinellas County at the Woodlawn site, AQS Site # 12-103-0012. Site reviews conducted from 2015 through 2020 found that the siting requirements in 40 CFR Part 58 Appendix E, Table E-4 could not be met. The most recent site review information is provided in Table 5.5.

The site is on the edge of the neighborhood adjacent to an industrial area just west of the site, where elevated PM₁₀ concentrations would not be unusual, especially due to its proximity to a cement plant (Carroll's Building Materials). There is unrestricted airflow 270° around the sampler and the tree in question is to the east, therefore it does not impact the direction of concern. The tree is located on the St. Petersburg Parks Department's property and requests for the removal of the tree were denied.

The site has been in operation since 1992 and Pinellas county would prefer to continue operation of the site to meet local interests. Data collected pre- and post-discovery of siting issues correlate well and show negligible variability for the PM₁₀ concentrations. Additionally, the weighted annual averages for the Woodlawn and Davis Island sites demonstrates similar and consistent PM₁₀ concentrations within the last 10 years (see Table 5.6 below), with no exceedances of the PM₁₀ NAAQS.

Table 5.1 2020 Site Review of Woodlawn - AQS Site #12-103-0012

	Woodlawn Site
AQS Site #	12-103-0012
City (CBSA)	St. Petersburg
Site Name	Woodlawn
Statement of Purpose	Needed by Regulation
Site Review Date	10/20/2020
County	Pinellas
Location Latitude	27.785556 N
Location Longitude	-82.658333 W
Address	1313 19th St. N.
Objective	High Concentration
Pollutants Monitored	PM ₁₀
Sampling and Analysis Method	eBAM Plus, Continuous
Spatial Scale	Neighborhood
Operating Schedule	Continuous
Network Type	SLAMS
Distance from Inlet to nearest:	Wall/Inlet = 29 meters Tree Dripline = 9 meters Road = 5.7 meters
Access	Unlimited
Inlet Height	2.3 meters
Comments	Located on a platform beside 19th Street North. Distance from trees within 10 meters; does not meet siting criteria.

Figure 5.1 Street View of Woodlawn



Figure 5.2 East of Woodlawn Site




Table 5.6 PM₁₀ Weighted Annual Averages Woodlawn (12-103-0012) and Davis Island (12-057-1035) in µg/m³

Year	PM ₁₀ C (AQS Site#: 12-057-1035)	PM ₁₀ M ² (AQS Site#: 12-103-0012)	PM ₁₀ C ² (AQS Site#: 12-103-0012)
2009	20.6	21.1	N/A
2010	21.4	21.0	N/A
2011	20.2	17.6	N/A
2012	20.5	17.5	N/A
2013	19.7 ¹	16.1	N/A
2014	19.5	17.3	N/A
2015	18.6	18.3	N/A
2016	19.5	16.5	N/A
2017	19.7 ¹	19.8	N/A
2018	18.8 ¹	22.7	N/A
2019	19.3	N/A	17.0
2020	20.6	N/A	18.4

¹ There was insufficient data to produce a valid average

² The PM₁₀ monitor at Woodlawn was upgraded from a PM₁₀ Manual to a PM₁₀ Continuous monitor on January 1, 2019.

Figure 5.4 Woodlawn Site and PM₁₀ Source

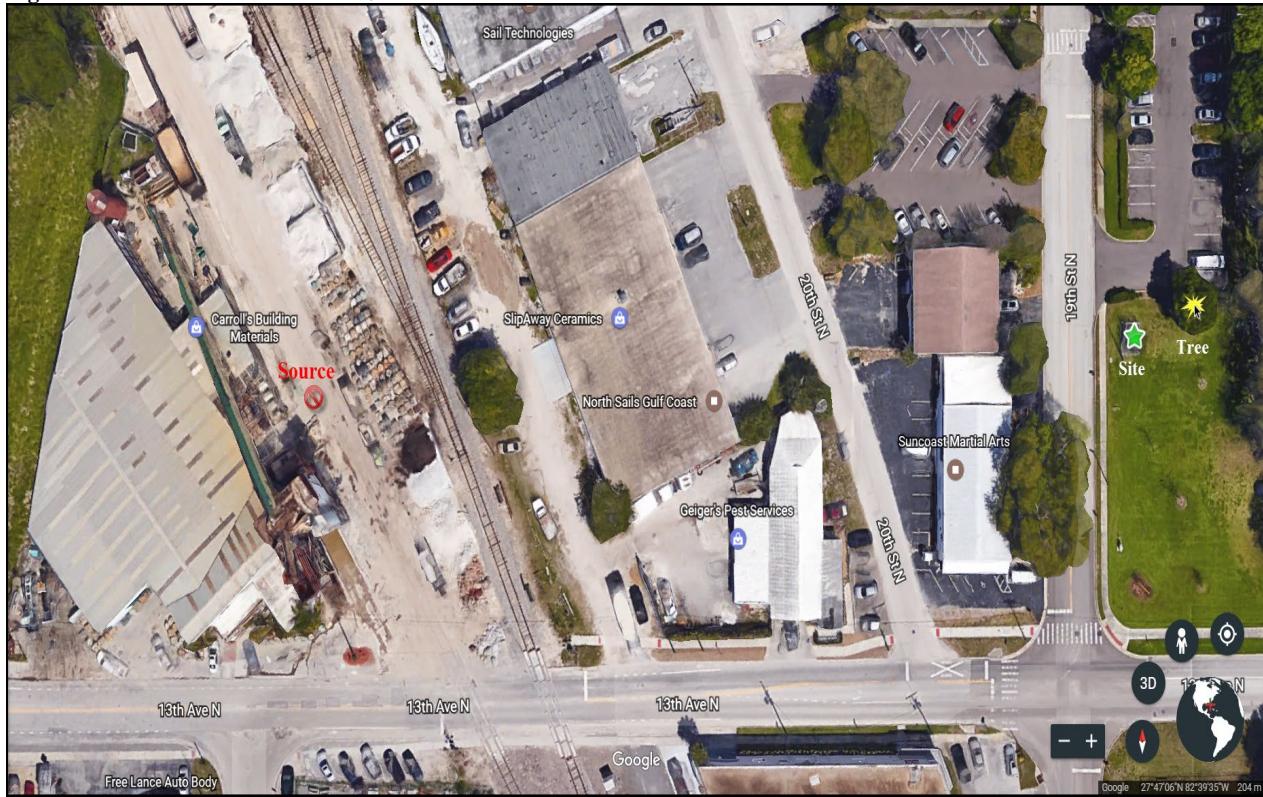

6.0 GLOSSARY OF AIR MONITORING TERMS

AADT	Annual Average Daily Traffic
AAMNAG	Ambient Air Monitoring Network Assessment Guidance
AQI	Air Quality Index – EPA's standardized method of reporting air quality information and forecast to the public.
AQS	Air Quality System – EPA's repository of ambient air quality data.
BAM	Beta Attenuation Mass Monitor – a type of continuous PM _{2.5} monitor.
CBSA	Core Based Statistical Area – a collective term for both metropolitan (metro) and micropolitan (micro) statistical areas.
CFR	Code of Federal Regulations
CO	Carbon monoxide – an odorless, colorless gaseous; one of the "Six Common Air Pollutants," also known as "Criteria Pollutants," regulated by EPA.
FE-AADT	Fleet Equivalent Annual Average Daily Traffic – a value calculated according to the NO ₂ near-road technical assistance document, which weighs heavy-duty traffic 10 times more than other vehicles.
FEM	Federal Equivalence Method – method approved for comparison to NAAQS.
FRM	Federal Reference Method – method approved for comparison to NAAQS.
IMPROVE	Interagency Monitoring of Protected Visual Environments
MSA	Metropolitan Statistical Area – a "geographic entity defined by the U.S. Office of Management and Budget (OMB) for use by federal statistical agencies in collecting, tabulating, and publishing Federal statistics." A MSA consists of a core urban area of at least 50,000 people.
NAAQS	National Ambient Air Quality Standards – maximum threshold concentrations above which adverse health effects may occur. EPA established NAAQS for Criteria Pollutants based on the 1970 Clean Air Act.
NATTS	National Air Toxics Trends Stations
NCore	National Core multi-pollutant monitoring stations – a collection of monitors that integrates several advanced measurement systems for particles, pollutant gases and meteorology.
NEI	National Emissions Inventory
NO	Nitrogen oxide
NO ₂	Nitrogen dioxide – a by-product of incomplete combustion that is intimately involved in photochemistry and ozone formation, as well as acid rain formation.
NO _x	A measure of total oxides of nitrogen, consisting primarily of nitrogen dioxide (NO ₂) and nitric oxide (NO).
NO _y	Total reactive nitrogen – a collective name for oxidized forms of nitrogen in the atmosphere, such as nitric oxide (NO), nitrogen dioxide (NO ₂), nitric acid (HNO ₃) and organic nitrates.
O ₃	Ozone – a gaseous pollutant and a component of smog at ground level; one of the "Six Common Air Pollutants," also known as "Criteria Pollutants," regulated by EPA.
PAMS	Photochemical Assessment Monitoring Station
PM	Particulate Matter – also known as particle pollution.
PM _{2.5}	Particulate Matter 2.5 micrometers in diameter and smaller.
PM ₁₀	Particulate Matter 10 micrometers in diameter and smaller.
PM _{10-2.5}	Particle size between 10 and 2.5.
PQAO	Primary Quality Assurance Organization
PWEI	Population Weighed Emissions Index
PSD	Prevention of Significant Deterioration
SIP	State Implementation Plan
SLAMS	State and Local Air Monitor Stations
SO ₂	Sulfur dioxide
SPM	Special Purpose Monitors
STN	Speciation Trends Network
SU/SD	Set-up/ Shut-down

7.0 APPENDICES

APPENDIX A: ADDITIONAL NETWORK INFORMATION

This appendix provides additional information to facilitate a full evaluation of several relocations within Florida's air monitoring network.

A.1 Site Relocations

➤ Homestead Fire Station Site: AQS Site # 12-086-6001

The Homestead Fire Station Site (AQS Site #: 12-086-6001), hereafter known as the Wittkop Park Site, will be located 704 meters northwest of its original location due structural integrity issues with the building. The new shelter will be located on the Homestead Public Services property and assigned a new AQS site identification number (12-086-6002) due to the change in address.

Photos and Wind Rose for the Miami-Dade County: Proposed Wittkop Park Site - AQS # 12-086-6002

Figure 7.1 North from Proposed Wittkop Park Site



Figure 7.2 South from Proposed Wittkop Park Site

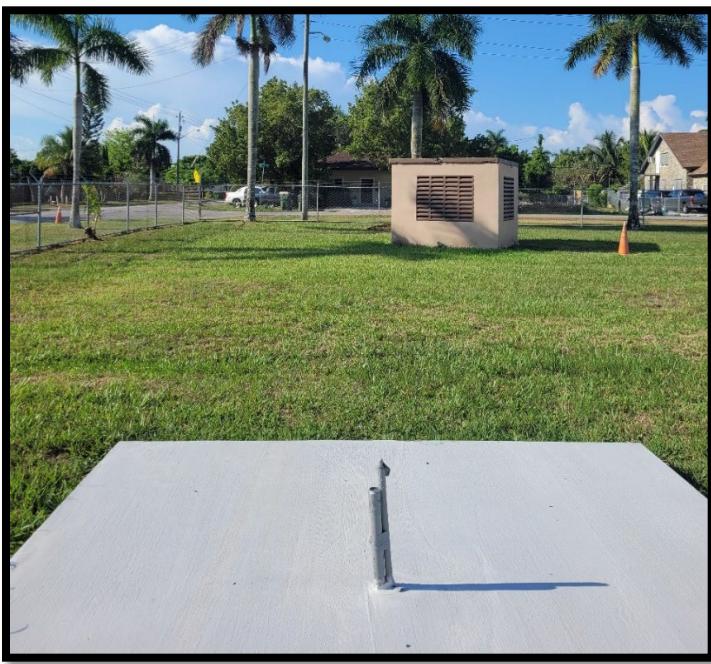


Figure 7.3 East from Proposed Wittkop Park Site



Figure 7.4 West from Proposed Wittkop Park Site



Figure 7.5 Aerial of Proposed Wittkop Park Site


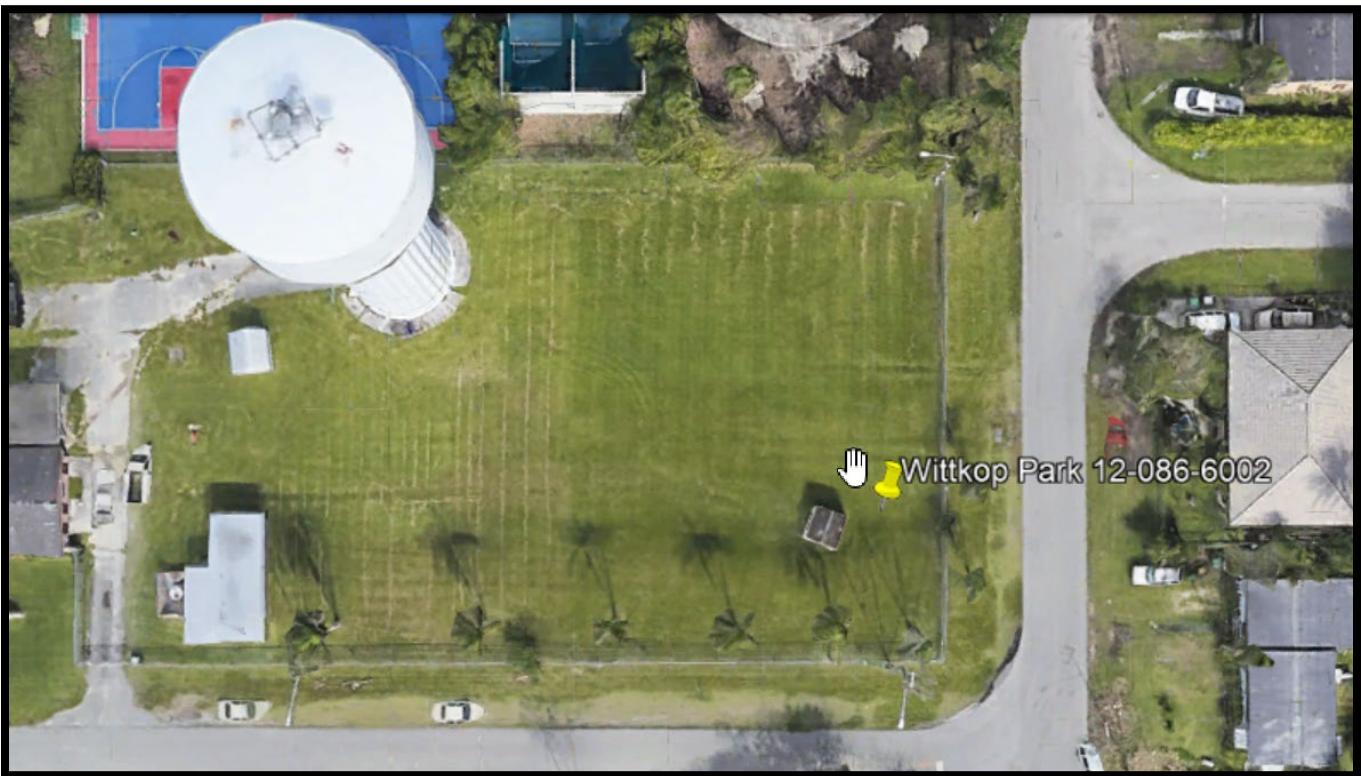


Figure 7.6 Wind Rose from Wittkop (AQS Site 12-086-6002)

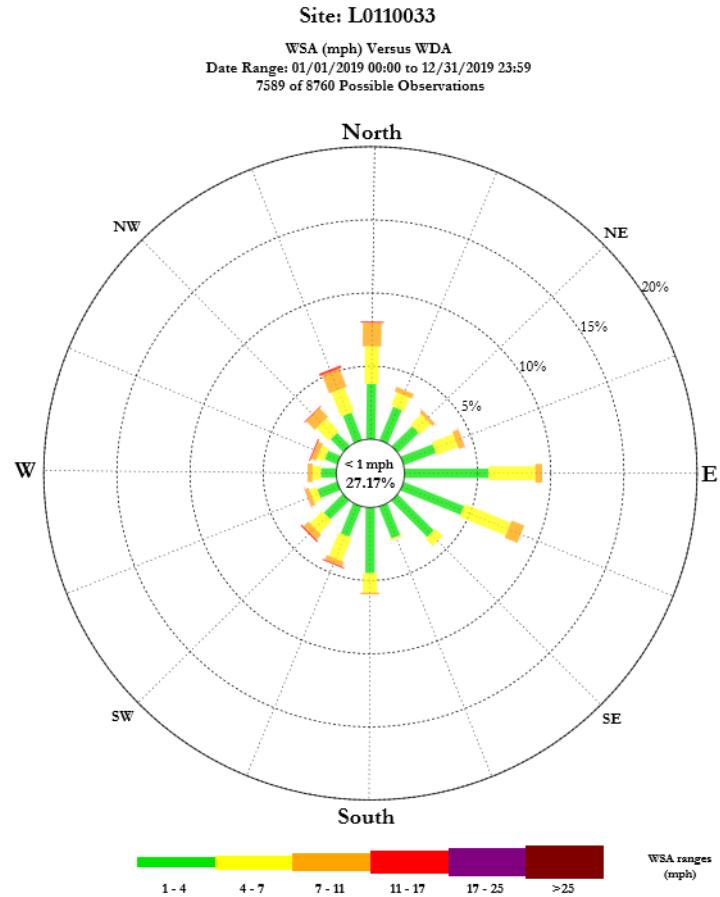

➤ **Winter Park: AQS Site # 12-095-2002**

The Winter Park Site (AQS Site #: 12-095-2002) will be relocated 192 meters SW of its original location on the property due to landlord (City of Winter Park) request. The site remains representative of the area's air mass and will retain its AQS Site number.

Photos and Wind Rose for the Orange County: Winter Park Site - AQS # 12-095-2002

Figure 7.7 North from Proposed Winter Park Site



Figure 7.8 East from Proposed Winter Park Site



*NOTE: Palm trees east of the new Winter Park site are being removed from the drip line

Figure 7.9 South from Proposed Winter Park Site




Figure 7.10 West from Proposed Winter Park Site



Figure 6.11 Aerial of Winter Park



Figure 6.12 Wind Rose from Winter Park Site

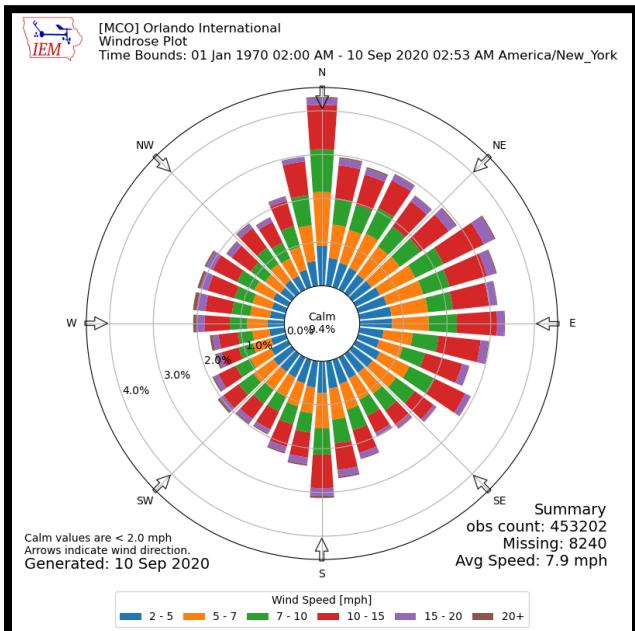

A.2 Temporary Discontinuance

➤ I-4 Near Road: AQS Site # 12-095-0009

The I-4 Near Road Site (AQS Site # 12-095-0009) was granted approval July 24, 2017 by EPA for a temporary discontinuance due to construction. A site visit was done by EPA during Orange County's Technical System Audit in 2020. Provided below are pictures of the construction taken June 2020 (see Figures 4.9 and 4.10)

Figure 4.9 I-4 Construction Update June 2020



Figure 4.10 I-4 Construction Update June 2020



APPENDIX B: ANNUAL SITE REVIEW SUMMARY

The Florida DEP's audit staff conduct site reviews to verify that sites meet probe line siting criteria. Identified issues are resolved as quickly as practicable. The date of the most recent site review, notes as to whether there are existing issues, and any comments regarding these issues are provided in the table below.

AQS #	Site Name	Agency	Parameters	Site Review Date	Issues Found (Y/N)	Issue Description (If Applicable)
12-001-3012	PAYNES PRAIRIE FARM	Nature Coast (44)	Oz, Cont PM2.5	1/27/2021	N	
12-003-0002	OLUSTEE	First Coast (48)	Oz, Cont. PM2.5	7/28/2020	N	
12-005-0006	ST ANDREWS STATE PARK	Emerald Coast (42)	Oz, Cont PM2.5	4/13/2021	N	
12-009-0007	MELBOURNE	Space Coast (47)	Oz, FRM PM2.5, Cont PM2.5, Cont PM10	1/25/2021	N	
12-009-4001	COCOA BEACH	Space Coast (47)	Oz	4/19/2021	N	
12-011-0033	VISTA VIEW	Broward County PPRAQD (17)	Oz, Cont PM2.5, Toxics	10/27/2020	N	
12-011-0034	BANU	Broward County PPRAQD (17)	Oz, PM10 (2), FRM PM2.5 (2), Cont PM2.5, TCO, TSO2, NOY, SASS, URG, Low Vol PM10, Toxics	10/28/2020	N	
12-011-0035	FORT LAUDERDALE NEAR ROAD	Broward County PPRAQD (17)	NO2, CO, Cont Pm2.5, Ultrafine, Toxics	6/19/2021	N	
12-011-2003	POMPANO HIGHLANDS	Broward County PPRAQD (17)	Oz, Cont. PM2.5	10/27/2020	N	
12-011-5005	COCONUT CREEK PARK	Broward County PPRAQD (17)	Cont. PM10, Cont. PM2.5	10/26/2020	N	
12-011-8002	Dr. VON MIZELL-EULA JOHNSON (FORMERLY JOHN U. LLOYD)	Broward County PPRAQD (17)	Oz, NO2	2/16/2021	N	
12-017-0006	CRYSTAL RIVER PRESERVE	Nature Coast (44)	SO2, Cont PM2.5	6/16/2021	N	
12-021-0004	LAUREL OAKS ELEM	Lee Island Coast (46)	Oz, Cont PM2.5	3/3/2021	N	
12-023-0002	VETERANS DOMICILE	First Coast (48)	Oz, Cont PM2.5	1/6/2021	N	

12-031-0032	KOOKER PARK	City of Jacksonville EQD (11)	SO2, NO2, FRM PM2.5, Cont PM10	2/3/2021	N	
12-031-0077	SHEFFIELD	City of Jacksonville EQD (11)	Oz, Cont PM2.5, Toxics	5/18/2021	Y	Trees too tall to the northwest and east; agency is working on resolving the issue.
12-031-0081	CEDAR BAY RD.	City of Jacksonville EQD (11)	SO2	3/22/2021	N	
12-031-0098	MANDARIN	City of Jacksonville EQD (11)	FRM PM2.5, Cont PM2.5	5/18/2021	N	
12-031-0099	SUNNY ACRES PARK	City of Jacksonville EQD (11)	FRM PM2.5 (2)	7/20/2020	N	
12-031-0100	MAYO CLINIC	City of Jacksonville EQD (11)	Oz, Cont PM2.5, Toxics	7/21/2020	N	
12-031-0106	CISCO DRIVE	City of Jacksonville EQD (11)	Oz	2/1/2021	N	
12-031-0108	PEPSI PLACE	City of Jacksonville EQD (11)	NO2, CO, Cont PM2.5 & PM10	5/17/2021	N	
12-033-0004	ELLYSON IND. PARK	Naval Aviation Coast (41)	Oz, SO2, Cont PM10, Cont PM2.5	1/5/2021	N	
12-033-0018	PENSACOLA NAS	Naval Aviation Coast (41)	Oz	7/28/2020	N	
12-035-0004	FLAGLER	Space Coast (47)	Oz	8/11/2020	N	
12-047-0015	WHITE SPRINGS	First Coast (48)	SO2, Cont PM2.5	1/6/2021	N	
12-055-0003	ARCHBOLD	Lee Island Coast (46)	Oz	1/12/2021	N	
12-057-0081	SIMMONS PARK	Hillsborough County EPC (12)	OZ	10/14/2020	N	
12-057-0083	GARDINIER	Hillsborough County EPC (12)	Cont PM10	4/21/2021	N	
12-057-0100	KENLY	Hillsborough County EPC (12)	Pb	10/6/2020	N	

12-057-0109	EAST BAY	Hillsborough County EPC (12)	SO2	2/17/2021	N	
12-057-0112	APOLLO BEACH	Hillsborough County EPC (12)	SO2, Cont PM2.5	2/16/2021	N	
12-057-0113	MUNRO STREET	Hillsborough County EPC (12)	TNO2, TCO, Cont PM2.5	6/22/2021	N	
12-057-1035	DAVIS ISLAND	Hillsborough County EPC (12)	Oz, SO2, Cont PM10	10/6/2020	N	
12-057-1065	GANDY	Hillsborough County EPC (12)	Oz, NO2, Cont PM2.5	4/20/2021	N	
12-057-1066	GULF COAST LEAD	Hillsborough County EPC (12)	Pb (2)	4/21/2021	N	
12-057-1073	PATENT	Hillsborough County EPC (12)	Pb	10/6/2020	N	
12-057-3002	SYDNEY	Hillsborough County EPC (12)	Oz, NOy, TSO2, TCO, Cont PM2.5, FRM PM2.5 (2), PM10 (2), Low Vol PM10, PM10/Puff, SASS, URG, Toxics, Summa, ERG, Aromatic Hydrocarbon	3/16/2021	N	
12-059-0004	BONIFAY TRI-COUNTY AIRPORT	Emerald Coast (42)	Oz, Cont PM2.5	10/26/2020	N	
12-069-0002	CLERMONT	Space Coast (47)	Oz	10/13/2020	Y	The tree to the northwest is too tall and less than 10 meters; agency is working on resolving the issue.
12-071-0005	FT MYERS WTP	Lee Island Coast (46)	FRM PM2.5, Cont PM2.5, Cont PM10	1/11/2021	N	
12-071-2002	CAPE CORAL	Lee Island Coast (46)	Oz	9/22/2020	N	
12-071-3002	FT. MYERS BEACH	Lee Island Coast (46)	Oz	4/28/2021	N	

12-073-0012	TALLAHASSEE CC	Forgotten Coast (43)	Oz, FRM PM2.5 (2), Cont PM2.5, SASS, URG, RADNET	5/11/2021	N	
12-081-0028	PORT MANATEE (DEP SO2)	Sun Coast (45)	SO2	4/27/2021	N	
12-081-3002	PORT MANATEE	Manatee County EMD (14)	Oz	8/31/2020	N	
12-081-4012	GT BRAY PARK	Manatee County EMD (14)	Oz	9/1/2020	N	
12-081-4013	39TH STREET	Manatee County EMD (14)	Oz	9/2/2020	N	
12-083-0003	OCALA YMCA	Nature Coast (44)	Oz, Cont PM2.5	6/15/2021	N	
12-083-0004	MARION CO SHERIFF	Nature Coast (44)	Oz	10/20/2020	N	
12-085-0007	STUART	Space Coast (47)	Oz, Cont PM2.5	1/27/2021	N	
12-086-0019	PENNSUCO	Miami-Dade County RER (18)	SO2	2/9/2021	N	
12-086-0027	ROSENSTIEL	Miami-Dade County RER (18)	Oz, NO2	11/30/2020	Y	The inlets are above 15 meters; waiver request included in this plan
12-086-0029	PERDUE	Miami-Dade County RER (18)	Oz, Toxics	5/26/2021	N	
12-086-0033	PALM SPRINGS	Miami-Dade County RER (18)	FRM PM2.5	2/8/2021	N	
12-086-0034	KENDALL	Miami-Dade County RER (18)	PM2.5	2/9/2021	N	
12-086-0035	PERIMETER ROAD	Miami-Dade County RER (18)	NO2	6/22/2021	N	
12-086-1016	MIAMI FIRE STATION	Miami-Dade County RER (18)	FRM PM2.5 (2), Cont PM2.5, PM10 (2)	12/1/2020	N	
12-086-4002	OLD LAB ANNEX	Miami-Dade County RER (18)	NO2, CO	11/3/2020	N	
12-086-6001	HOMESTEAD	Miami-Dade County RER (18)	FRM PM2.5, Cont PM2.5	11/4/2020	N	

12-086-6002	WITTKOPP PARK	Miami-Dade County RER (18)	Cont PM2.5	12/02/2020	N	
12-089-0005	FERNANDINA BEACH	First Coast (48)	SO2	1/5/2021	N	
12-091-0002	FT WALTON BEACH	Emerald Coast (42)	Oz, Cont PM10	10/27/2020	N	
12-095-0010	SKYVIEW	Orange County EPD (20)	Oz	10/15/2020	N	
12-095-0009	I-4	Orange County EPD (20)	NO2, CO, Cont PM2.5	N/A	N	Temporarily Shut Down
12-095-2002	WINTER PARK	Orange County EPD (20)	Oz, NO2, SO2, CO, FRM PM2.5 (2), PM10 (2), Cont PM2.5, Summa, Carbonyl	2/9/2021	N	Location before relocation
12-097-2002	KISSIMMEE FIRE	Space Coast (47)	Oz	10/12/2020	Y	Trees to the northwest and southeast are too tall. Crowns of trees need to be reduced; agency is working on resolving the issue.
12-099-0008	BELLE GLADE	Palm Beach County EPH (16)	Cont PM2.5	4/26/2021	N	
12-099-0021	LANTANA SCRUB PRESERVE	Palm Beach County EPH (16)	Oz	4/26/2021	N	
12-099-0022	Lamstein Lane	Palm Beach County EPH (16)	Oz, FRM PM2.5 (2), Cont PM10	11/17/2020	N	
12-099-2005	DELRAY BEACH	Palm Beach County EPH (16)	FRM PM2.5, cont. PM10.	11/16/2020	N	
12-101-0005	SAN ANTONIO	Sun Coast (45)	Oz	4/28/2021	N	
12-101-2001	HOLIDAY	Sun Coast (45)	Oz	3/24/2021	N	
12-103-0004	ST. PETERSBURG COLLEGE	Pinellas County AQD (13)	Oz	3/2/2021	N	

12-103-0012	WOODLAWN (Pinellas)	Pinellas County AQD (13)	PM10	10/20/2020	Y	Tree dripline issue; waiver request included in this plan
12-103-0018	AZALEA PARK	Pinellas County AQD (13)	Oz, NO2, PM10 Cont, Cont PM2.5, VOC	12/8/2020	N	
12-103-0023	DERBY LANE	Pinellas County AQD (13)	SO2	10/21/2020	N	
12-103-0027	SAWGRASS LAKE	Pinellas County AQD (13)	NO2, CO, Aethelometer	6/8/2021	N	
12-103-3004	COUNTY MOTORPOOL	Pinellas County AQD (13)	PM10 Cont	10/21/2020	N	
12-103-5002	EAST LAKE	Pinellas County AQD (13)	Oz, Cont PM2.5, PM10	5/25/2021	N	
12-103-5003	OAKWOOD	Pinellas County AQD (13)	SO2	5/25/2021	N	
12-105-6005	SIKES ELEMENTARY	Sun Coast (45)	Oz, SO2	9/21/2020	N	
12-105-6006	BAPTIST CHILD HOME	Sun Coast (45)	Oz, FRM PM2.5 (2), Cont PM2.5, Cont PM10	3/23/2021	N	
12-107-1008	PALATKA BARGE PORT	Nature Coast (44)	SO2, Cont PM10	1/26/2021	N	
12-111-0013	SAVANNAS	Space Coast (47)	Oz	1/27/2021		
12-113-0015	WOODLAWN BEACH MIDDLE	Naval Aviation Coast (41)	Oz, Cont PM2.5	1/6/2021	N	
12-115-0013	BEE RIDGE	Sarasota County AWQD (15)	FRM PM2.5, Cont PM2.5	9/14/2020	N	
12-115-1005	LIDO PARK	Sarasota County AWQD (15)	Oz	10/6/2020	N	
12-115-1006	PAW PARK	Sarasota County AWQD (15)	Oz, NO2, Cont PM10	10/6/2020	N	
12-115-2002	JACKSON ROAD	Sarasota County AWQD (15)	Oz, Cont PM2.5	6/15/2021	N	
12-117-1002	SEMINOLE CC	Space Coast (47)	Oz, FRM PM2.5, Cont	4/20/2021	N	

			PM2.5, Cont PM10			
12-127-5002	DAYTONA BEACH	Space Coast (47)	Oz, FRM PM2.5, Cont PM2.5, Cont PM10	8/12/2020	N	
12-129-0001	ST MARKS WILDLIFE	Forgotten Coast (43)	Oz, NOy, TSO2, TCO, Cont PM2.5	2/4/2021	N	

¹Includes site reviews conducted as of June 15, 2021.

*Primary and collocated monitor.

APPENDIX C: AMBIENT AIR MONITORING NETWORK DESCRIPTION

Florida's air monitoring network, including changes expected through June 30, 2019, is described in Appendix C. It is organized by Metropolitan Statistical Area from largest to smallest.

Florida Ambient Air Monitoring Network Description

METROPOLITAN STATISTICAL AREA: MIAMI - FT LAUDERDALE - MIAMI BEACH (BROWARD, MIAMI-DADE AND PALM BEACH COUNTIES)												
Broward County												
AQS #	SITE NAME	ADDRESS/ COORDINATES	TYPE	POLLUTANT	POC	OPERATING SCHEDULE	SAMPLER	MONITORING OBJECTIVE	SPATIAL SCALE	STATEMENT OF PURPOSE	MODIFICATIONS	COMMENTS
12-011-0033	Vista View Park	4001 SW 142 Ave, Davie, FL 33330; 26.073056, -80.338889	SLAMS	Ozone	1	Continuous	Thermo 49i	POP EXP	NBH	TRENDS MONITORING		SU 7/1/2008
			SPM	PM _{2.5}	3	Continuous	MET One BAM 1020	POP EXP	NBH	TRENDS MONITORING	REPLACE BY FEM	SU 1/28/2009 REPLACEMENT EXPECTED 10/1/2021
			SLAMS	PM _{2.5}	3	Continuous	Teledyne T640	POP EXP	NBH	TRENDS MONITORING	ADD	SU EXPECTED 10/1/2021
12-011-0034	Daniela Banu (NCore Site)	5300 S. Pine Island Rd., Davie, FL 33328; 26.0538889, -80.256944	SLAMS	CO	1	Continuous	Thermo 48C-TLE	POP EXP	NBH	NEEDED BY REGULATION		SU 7/1/2015; Trace Level;
			SLAMS	SO ₂	1	Continuous	Thermo 43i-TLE	POP EXP	NBH	NEEDED BY REGULATION		SU 7/1/2015; Trace Level
			SLAMS	Ozone	1	Continuous	Thermo 49i	POP EXP	NBH	NEEDED BY REGULATION		SU 7/1/2015
			SLAMS	PM ₁₀	3	Continuous	Teledyne 640X	POP EXP	NBH	NEEDED BY REGULATION		SU 10/2019; FEM
			SLAMS	PM _{2.5}	1	Every 3rd Day	Thermo 2025i	POP EXP	NBH	NEEDED BY REGULATION		SU 1/1/2015
			SLAMS	PM _{2.5}	3	Continuous	Teledyne T640X	POP EXP	NBH	NEEDED BY REGULATION		SU 09/1/2019; FEM
			SLAMS	PMCoarse	1	Continuous	Teledyne T640X	POP EXP	NBH	NEEDED BY REGULATION		SU 10/1/2019
			SLAMS	NO _y	1	Continuous	Thermo 42i-Y	POP EXP	NBH	NEEDED BY REGULATION		SU 7/1/2015; Trace Level
			SLAMS	SPEC. PM _{2.5}	5	Every 6th Day	MET One SASS	POP EXP	NBH	TRENDS MONITORING		SU 1/1/2015
			CSN	EC/OC		Every 3rd Day	URG 3000N	POP EXP	NBH	TRENDS MONITORING		SU 1/1/2015
			NON-REG	Toxics		Every 6th Day	ATEC 2200	POP EXP	NBH	BASELINE MONITORING		SU 11/1/2015
			NON-REG	Meteorology		Continuous	RM Young Wind Speed/Wind Direction	POP EXP	NBH	SUPPORT NCORE NETWORK		SU 01/1/2020
			NON-REG	Meteorology		Continuous	RM Young 41382 VC T/ RH Sensor	POP EXP	NBH	SUPPORT NCORE NETWORK	REPLACE	SU 01/1/2020; REPLACED by 41342VC EXPECTED 6/1/2021
12-011-0035	Fort Lauderdale Near Road	799 N I-95, Ft. Lauderdale, FL 33311; 26.131256, -80.167847	SLAMS	CO	1	Continuous	Thermo 48i-TLE	POP EXP	URBAN	NEEDED BY REGULATION		SU 8/1/2015; Trace level
			SLAMS	NO ₂	1	Continuous	Teledyne T200UP	POP EXP	URBAN	NEEDED BY REGULATION		SU 8/1/2015; Near-road Site
			SLAMS	PM _{2.5}	3	Continuous	Teledyne T640	POP EXP	URBAN	NEEDED BY REGULATION		SU 8/1/2015; FEM
			SLAMS	BC	1	Continuous	Teledyne API 633	POP EXP	URBAN	NEEDED BY REGULATION		SU 1/20/2017
			SLAMS	UFP	1	Continuous	TSI 3031	POP EXP	URBAN	NEEDED BY REGULATION		SU 3/15/2017
			SLAMS	WD/WS	1	Continuous	RM Young 8100	POP EXP	URBAN	NEEDED BY REGULATION	ADD	SU EXPECTED 07/01/2021
12-011-2003	Pompano Highland Fire House	1951 NE 48th Street, Pompano Beach, FL 33060; 26.290765, -80.096665	SLAMS	Ozone	1	Continuous	Thermo 49i	POP EXP	NBH	RELIED ON SPATIAL COVERAGE		SU 1/1/1989
			SLAMS	PM _{2.5}	3	Continuous	Teledyne T640	POP EXP	NBH	INTERPOLATION		SU 4/1/2019; FEM
12-011-5005	Coconut Creek	5005 Winston Park Blvd, Coconut Creek, FL 33073; 26.294167, -80.176389	SLAMS	PM ₁₀	1	Continuous	MET One eBAMS+	POP EXP	NBH	SOURCE MONITORING	REPLACE BY FEM	SU 1/1/2018; FEM REPLACEMENT EXPECTED 10/2021
			SLAMS	PM _{2.5}	3	Continuous	Teledyne T640	POP EXP	NBH	NEEDED BY REGULATION	REPLACE BY FEM	SU 1/1/2019; FEM REPLACEMENT EXPECTED 10/2021
			SLAMS	PM ₁₀	3	Continuous	Teledyne T640X	POP EXP	NBH	NEEDED BY REGULATION	ADD	SU EXPECTED 10/1/2021
			SLAMS	PM _{2.5}	3	Continuous	Teledyne T640X	POP EXP	NBH	NEEDED BY REGULATION	ADD	SU EXPECTED 10/1/2021
12-011-8002	Dr. Von Mizell-Eula Johnson State Park	7000 N. Ocean Dr., Dania, FL 33004; 26.087198, -80.111415	SLAMS	NO ₂	1	Continuous	Thermo 42i	POP EXP	NBH	COMM-WIDE MONITORING		SU 7/8/1990
			SLAMS	Ozone	1	Continuous	Thermo 49i	HI CONC	NBH	NEEDED BY REGULATION		SU 1/1/1985
Miami-Dade County												
AQS #	SITE NAME	ADDRESS/ COORDINATES	TYPE	POLLUTANT	POC	OPERATING SCHEDULE	SAMPLER	MONITORING OBJECTIVE	SPATIAL SCALE	STATEMENT OF PURPOSE	MODIFICATIONS	COMMENTS
12-086-0019	Pennsuco	14001-14027 N Okeechobee Rd, Hialeah, FL 33018; 25.899167, -80.382778	SLAMS	SO ₂	1	Continuous	Thermo 43i	POP EXP	NBH	TRENDS MONITORING		SU 8/18/1987
12-086-0027	Rosentiel (University of Miami)	4600 Rickenbacker Causeway, Miami, FL 33149; 25.732500, -80.161944	SLAMS	NO ₂	1	Continuous	Teledyne T200	POP EXP/ UPWIND BKGD	NBH	VULNERABLE AND SUSCEPTIBLE MONITORING		SU 1/30/1985
			SLAMS	Ozone	1	Continuous	Thermo 49i	POP EXP/ UPWIND BKGD	NBH	NEEDED BY REGULATION		SU 3/7/1984

12-086-0029	Perdue	19590 Old Cutler Rd, Cutler Ridge, FL 33157; 25.586944, -80.326111	SLAMS	Ozone	1	Continuous	Thermo 49i	HI CONC	URBAN	USED FOR AQI		SU 5/1/1985
12-086-0033	Palm Springs Fire Station	7700 NW 186th St, Palm Springs, FL 33015; 25.941944, -80.326388	SLAMS	PM _{2.5}	1	Every 3rd Day	Thermo 2025i	POP EXP	NBH	MONITORING GROWTH IMPACT		SU 5/4/2005
12-086-0034	Kendall	9015 SW 127th Ave, Miami, FL 33186; 25.683330, -80.399722	SPM	PM _{2.5}	1	Continuous	Thermo 1405	POP EXP	MIDDLE	USED FOR AQI		SU 7/1/2018
12-086-0035	Perimeter Road	5600 Perimeter Road, Miami, FL 33126; 25.7854722, -80.2842055	SLAMS	NO ₂	1	Continuous	Teledyne T200	SOURCE	MICRO	NEEDED BY REGULATION		SU 1/11/2016; Near-road Site
12-086-1016	Miami Fire Station	1200 NW 20th St, Miami, FL 33142; 25.794722, -80.215556	SLAMS	PM _{2.5}	2	Every 12th Day	Thermo 2025i	HI CONC	NBH	QA COLLOCATION		SU 2/4/1999; Collocated monitor
			SLAMS	PM _{2.5}	3	Continuous	Teledyne T640X	POP EXP	NBH	NEEDED BY REGULATION		SU 4/1/2018; FEM
			SLAMS	PM ₁₀	3	Continuous	Teledyne T640X	POP EXP	NBH	NEEDED BY REGULATION		SU 4/1/2018; FEM
12-086-4002	Lab Annex	864 NW 3rd St, Miami, FL 33127; 25.798333, -80.210278	SLAMS	CO	1	Continuous	Teledyne 300E	HI CONC	NBH	TRENDS MONITORING		SU 1/1/1976
12-086-6001	Homestead Fire Station	325 NW 2nd St, Homestead, FL 33030; 25.471944, -80.482778	SLAMS	PM _{2.5}	1	Every 3rd Day	Thermo 2025i	POP EXP	NBH	NEEDED BY REGULATION	SHUTDOWN	SU 1/27/1999; SD EXPECTED 10/2021
			SLAMS	PM _{2.5}	3	Continuous	Thermo 1400AB	POP EXP	NBH	USED FOR AQI	SHUTDOWN	SU 2/10/2004; SD EXPECTED 10/2021
12-086-6002	Wittkop Park	505 NW 9th Street, Homestead, FL 33030; 28.478249, -80.483754	SLAMS	PM _{2.5}	3	Continuous	Teledyne T640	POP EXP	NBH	NEEDED BY REGULATION	ADD	SU EXPECTED 10/2021 ; FEM

Palm Beach County

AQS #	SITE NAME	ADDRESS/COORDINATES	TYPE	POLLUTANT	POC	OPERATING SCHEDULE	SAMPLER	MONITORING OBJECTIVE	SPATIAL SCALE	STATEMENT OF PURPOSE	MODIFICATIONS	COMMENTS
12-099-0021	Lantana Preserve	968 N 8th St, Lantana, FL 33462; 26.5938083, -80.0584917	SLAMS	Ozone	1	Continuous	Thermo 49i	POP EXP	URBAN	NEEDED BY REGULATION		SU 2/2/2015
12-099-0022	Lamstein Lane	Lamstein Ln, Royal Palm Beach, FL 33411; 26.687606, -80.219619	SLAMS	Ozone	1	Continuous	Thermo 49i	HI CONC	NBH	NEEDED BY REGULATION		SU 1/15/2019; Relocation from 099-0009
12-099-0022	Lamstein Lane	Lamstein Ln, Royal Palm Beach, FL 33411; 26.687606, -80.219619	SLAMS	PM _{2.5}	1	Continuous	Thermo 5014i	POP EXP	NBH	NEEDED BY REGULATION		SU 1/17/2019; FEM, Relocation from 099-0009
12-099-0008	Belle Glade	38754 State Rd 80, Belle Glade, FL 33430; 26.724776, -80.666447	NON-REG	PM _{2.5}	3	Continuous	MET One BAM 1020	POP EXP	NBH	USED FOR AQI	REPLACED BY FEM	SU 5/1/2009; FEM; SD EXPECTED 06/2021
12-099-2005	Delray Beach	225 S. Congress Ave, Delray Beach, FL 33445; 26.456944, -80.092778	SLAMS	PM _{2.5}	3	Continuous	Teledyne T640	POP EXP	NBH	NEEDED BY REGULATION	ADD	SU EXPECTED 07/2021 ; FEM
			SLAMS	PM _{2.5}	1	Every 3rd Day	Thermo 2025i	POP EXP	NBH	NEEDED BY REGULATION	REPLACED BY FEM	SU 5/31/2001; SD 3/31/2021
			SLAMS	PM ₁₀	3	Continuous	MET One BAM 1020	POP EXP	NBH	NEEDED BY REGULATION	REPLACED BY ALTERNATE FEM	SU 02/03/2015; SD 3/31/2021
			SLAMS	PM _{2.5}	3	Continuous	Teledyne T640X	POP EXP	NBH	NEEDED BY REGULATION	ADD	SU 4/1/2021; FEM
			SLAMS	PM ₁₀	3	Continuous	Teledyne T640X	POP EXP	NBH	NEEDED BY REGULATION	ADD	SU 4/1/2021 ; FEM

METROPOLITAN STATISTICAL AREA: TAMPA - ST PETERSBURG - CLEARWATER (HILLSBOROUGH, PINELLAS, PASCO AND HERNANDO COUNTIES)

Pasco County												
AQS #	SITE NAME	ADDRESS/COORDINATES	TYPE	POLLUTANT	POC	OPERATING SCHEDULE	SAMPLER	MONITORING OBJECTIVE	SPATIAL SCALE	STATEMENT OF PURPOSE	MODIFICATIONS	COMMENTS
12-101-0005	San Antonio	30908 Warder Rd., San Antonio, FL 33576; 28.332225, -82.305643	SLAMS	Ozone	1	Continuous	Thermo 49i	POP EXP	URBAN	URBAN SPRAWL		SU 9/7/2000
12-101-2001	Holiday	3452 Darlington Rd., Holiday, FL 34691; 28.195574, -82.756264	SLAMS	Ozone	1	Continuous	Thermo 49i	HI CONC	URBAN	URBAN SPRAWL		SU 1/17/1992

Hillsborough County

12-057-0112	Apollo Beach	6506 Dolphin Cove Dr, Apollo Beach, FL 33572; 27.779712, -82.419835	SPM	SO ₂	1	Continuous	Thermo 43i	SOURCE	MICRO	NEEDED BY REGULATION		SU 1/1/2016
12-057-0113	Munro Street	1497 N. Munro Street, Tampa, FL 33607; 27.955550, -82.467140	SPM	PM _{2.5}	1	Continuous	Thermo 1405	SOURCE	MICRO	NEEDED BY REGULATION		SU 1/1/2016
			SLAMS	CO	1	Continuous	Thermo 48iQ TLE	SOURCE	MICRO	NEEDED BY REGULATION		SU 2/1/2016
			SLAMS	NO ₂	1	Continuous	Teledyne T200UP	SOURCE	MICRO	NEEDED BY REGULATION		SU 2/1/2016; Near-road Site
			SLAMS	PM _{2.5}	1	Continuous	Teledyne T640	SOURCE	MICRO	NEEDED BY REGULATION		SU 6/26/2019
			SPM	BC	1	Continuous	Magee AE-33	POPULATION EXPOSURE	MICRO	TRENDS MONITORING		SU 2/1/2016
12-057-0081	E.G. Simmons Park	2401 19th Avenue Northwest, Ruskin, FL 33570; 27.740033, -82.465146	SLAMS	Ozone	1	Continuous	Thermo 49i	HI CONC	URBAN	USED FOR AQI		SU 6/14/1978

12-057-0083	Gardiner Park	6501 Riverview Dr., Riverview, FL 33578; 27.864192, -82.384259	SPM	PM ₁₀	3	Continuous	Thermo 1405	SOURCE	MIDDLE	SOURCE MONITORING		SU 4/1/1995
12-057-0100	Kenly	2909 N 66th St, Tampa, FL 33619; 27.970328, -82.380050	SPM	Pb	1	Every 6th Day	Hi-Vol	SOURCE	MIDDLE	SOURCE MONITORING		SU 4/1/2010
12-057-0109	East Bay	9849 Highway 41 S., Gibsonton, FL 33534; 27.854176, -82.383728	SLAMS	SO ₂	1	Continuous	Thermo 43i	SOURCE	NBH	SOURCE MONITORING		SU 11/13/1996; Relocated on existing property 01/2020
12-057-1035	Davis Island (Coast Guard Station)	155 Columbia Dr., Tampa, FL 33606; 27.928356, -82.454539	SLAMS	SO ₂	1	Continuous	Thermo 43i	POP EXP	NBH	FOR EFFECTIVENESS OF NEW REGULATIONS		SU 1/1/1974
			SLAMS	Ozone	1	Continuous	Thermo 49i	POP EXP	NBH	USED FOR AQI		SU 1/1/1973
			SLAMS	PM ₁₀	1	Continuous	Thermo 1405	POP EXP	NBH	NEEDED BY REGULATION/USED FOR AQI		SU 12/1/1985
12-057-1065	USMC Reserve Center	5121 Gandy Blvd, Tampa, FL 33611; 27.89222,-82.538611	SLAMS	Ozone	1	Continuous	Thermo 49iQ	POP EXP	NBH	NEEDED BY REGULATION		SU 1/19/2019
12-057-1066	Gulf Coast Lead	1700 N. 66th St., Tampa, FL 33629; 27.960148, -82.381873	SPM	PM _{2.5}	3	Continuous	Thermo 1405	HI CONC	NBH	USED FOR AQI		SU 1/1/2004
			SLAMS	Pb	1	Every 6th Day	ANDERSEN 2000	SOURCE	MIDDLE	SOURCE MONITORING		SU 1/1/2009
12-057-1073	Patent Scaffolding	6811 E. 14th Avenue, Tampa, FL 33619; 27.96483,-82.37921	SPM	Pb	1	Every 6th Day	Tisch Hi-Vol	SOURCE	MIDDLE	SOURCE MONITORING		SU 1/1/2009
12-057-3002	Sydney (NCore Site)	1167 N. Dover Rd., Dover, FL 33527; 27.965650, -82.230400	SLAMS	CO	2	Continuous	Thermo 48i-TLE	POP EXP	URBAN	NEEDED BY REGULATION		SU 10/1/2005; Trace level
			SLAMS	SO ₂	1	Continuous	Thermo 43i-TLE	POP EXP	URBAN	NEEDED BY REGULATION		SU 1/1/2004; Trace Level
			SLAMS	NO _Y	1	Continuous	Thermo 42i-Y	POP EXP	URBAN	NEEDED BY REGULATION		SU 1/1/2004
			SLAMS	Ozone	1	Continuous	Thermo 49i	POP EXP	URBAN	NEEDED BY REGULATION		SU 1/1/2004
			SLAMS	PM _{2.5}	1	Every 3rd Day	Thermo 2025i	POP EXP	URBAN	NEEDED BY REGULATION		SU 1/1/2004
			SLAMS	PM _{2.5}	2	Every 12th Day	Thermo 2025i	POP EXP	URBAN	QA COLLOCATION		SU 1/26/2010; Collocated monitor
			SLAMS	PM _{2.5}	3	Continuous	Thermo 5014i	POP EXP	URBAN	USED FOR AQI		SU 2/14/2014; FEM
			SLAMS	PMCoarse	1	Every 3rd Day	Thermo 2025i	POP EXP	URBAN	NEEDED BY REGULATION		SU 1/1/2004
			STN	EC/OC		Every 3rd Day	URG 3000N	POP EXP	URBAN	BASELINE MONITORING		SU 1/1/2007
			STN	SPEC. PM _{2.5}		Every 3rd Day	MET One SASS	POP EXP	URBAN	TRENDS MONITORING		SU 1/1/2004
			NATTS	Toxics		Every 6th Day		POP EXP	URBAN	NEEDED BY REGULATION		SU 1/1/2004
				Meteorology		Continuous		POP EXP	URBAN	SUPPORT NCORE NETWORK		SU 1/1/2005
Pinellas County												
AQS #	SITE NAME	ADDRESS/COORDINATES	TYPE	POLLUTANT	POC	OPERATING SCHEDULE	SAMPLER	MONITORING OBJECTIVE	SPATIAL SCALE	STATEMENT OF PURPOSE	MODIFICATIONS	COMMENTS
12-103-0004	St. Petersburg College	2435 Sharkey Rd., Clearwater, FL 33765; 27.946688, -82.731767	SLAMS	Ozone	1	Continuous	Teledyne API T400	HI CONC	URBAN	NEEDED BY REGULATION		SU 7/1/1978
			SLAMS	PM _{2.5}	1	Continuous	Teledyne T640	POP EXP	NBH	NEEDED BY REGULATION		SU 3/20/2019
12-103-0012	Woodlawn	1313 9th St. N., St. Petersburg, FL 33713; 27.784749, -82.659265	SLAMS	PM ₁₀	1	Continuous	eBAM Plus	HI CONC	NBH	SOURCE MONITORING		SU 1/1/2019; FEM
12-103-0018	Azalea Park	7200-22 Ave N., St. Petersburg, FL 33701; 27.785866, -82.739875	SLAMS	NO ₂	1	Continuous	Teledyne T500U	HI CONC/ POP EXP	NBH	COMM-WIDE MONITORING		SU 1/1/1978
			SLAMS	Ozone	1	Continuous	Teledyne API T400	POP EXP	NBH	USED FOR AQI		SU 4/6/1978
			SLAMS	PM ₁₀	2	Continuous	Teledyne T640X	POP EXP	NBH	NEEDED BY REGULATION		SU 1/1/2018; FEM
			SLAMS	PM _{2.5}	3	Continuous	Teledyne T640X	POP EXP	NBH	NEEDED BY REGULATION		SU 1/1/2018; FEM
			NON-REG	Toxics		Every 6th Day		POP EXP	NBH	BASELINE MONITORING		SU 1/1/2001
12-103-0023	Derby Lane	10100 San Martin Rd., St. Petersburg, FL 33702; 27.863635, -82.623153	SLAMS	SO ₂	1	Continuous	Thermo 43i	POP EXP	NBH	TRENDS MONITORING		SU 1/14/1979
12-103-0026	Skyview	8601 60th Street N., Pinellas Park, FL 33702; 27.850041, -82.714590	NATTS	BC	1	Continuous	Teledyne API 633	POP EXP	NBH	BASELINE MONITORING		SU 5/20/2016
			NATTS	Toxics		Every 6th Day		POP EXP	NBH	BASELINE MONITORING		SU 05/20/2016
12-103-0027	Sawgrass Lake Park	6853 25th Street N., St. Petersburg, FL 33702; 27.834409, -82.665251	SLAMS	CO	1	Continuous	Teledyne T300U	SOURCE	MICRO	SUPPORT NEAR-ROAD		SU 5/20/2016
			SLAMS	NO ₂	1	Continuous	Teledyne T500U	SOURCE	MICRO	NEEDED BY REGULATION		SU 05/20/2016; Near-road Site
			SPM	BC	1	Continuous	Teledyne API 633	SOURCE	MICRO	SUPPORT NEAR-ROAD		SU 05/20/2016
12-103-3004	County Motorpool	1301 Ulterton Rd., Largo, FL 33771; 27.895856, -82.774546	SLAMS	PM ₁₀	3	Continuous	eBAM Plus	HI CONC	MIDDLE	TRENDS MONITORING		SU 1/1/2019
12-103-5002	John Chensut Sr. Park - East Lake	2200 East Lake Rd., Palm Harbor, FL 34685; 28.090299, -82.700707	SLAMS	Ozone	1	Continuous	Teledyne API T400	POP EXP	URBAN	USED FOR AQI		SU 1/1/1977
			SPM	PM _{2.5}	3	Continuous	Thermo 1405	POP EXP	NBH	USED FOR AQI		SU 9/5/2007

12-103-5003	Oakwood	40671 US 19 N., Tarpon Springs, FL 34689; 28.141667, -82.739722	SLAMS	SO ₂	1	Continuous	Thermo 43i	SOURCE	NBH	TRENDS MONITORING		SU 9/18/1998
METROPOLITAN STATISTICAL AREA: JACKSONVILLE (BAKER, CLAY, DUVAL, NASSAU AND ST. JOHNS COUNTIES)												
Baker County												
AQS #	SITE NAME	ADDRESS/ COORDINATES	TYPE	POLLUTANT	POC	OPERATING SCHEDULE	SAMPLER	MONITORING OBJECTIVE	SPATIAL SCALE	STATEMENT OF PURPOSE	MODIFICATIONS	COMMENTS
12-003-0002	Osceola National Forest - Olustee Ranger Station	Hwy 90, Olustee, Forest Service Office, Sanderson, FL 32087; 30.201111, -82.441111	SPM	Ozone	1	Continuous	Thermo 49i	POP EXP/ GEN BKGD	URBAN	REGIONAL BACKGROUND		SU 1/1/1996
			SPM	PM _{2.5}	3	Continuous	Thermo 1405	POP EXP	NBH	REGIONAL BACKGROUND		SU 02/2020
Duval County												
12-031-0032	Kooker Park	2900 Bennett St., Jacksonville, FL 32206; 30.355856, -81.635581	SLAMS	SO ₂	1	Continuous	Thermo 43i	HI CONC	NBH	TRENDS MONITORING		SU 1/1/1974
			SLAMS	NO ₂	2	Continuous	Thermo 42i	HI CONC	NBH	COMM-WIDE MONITORING		SU 1/6/1975
			SLAMS	PM ₁₀	1	Continuous	Thermo 1405	HI CONC	NBH	NEEDED BY REGULATION		SU 2/1/2008
			SPM	PM _{2.5}	1	Continuous	Thermo 1405	POP EXP	NBH	COMM RESPONSE		SU 7/1/2018
12-031-0077	Sheffield Elementary	13333 Lanier Rd., Jacksonville, FL 32226; 30.477275, -81.587167	SLAMS	Ozone	1	Continuous	Thermo 49i	POP EXP	NBH	NEEDED BY REGULATION		SU 1/1/1979
12-031-0081	Cedar Bay STP	1080 Cedar Bay Rd., Jacksonville, FL 32218; 30.431222, -81.631627	SLAMS	SO ₂	1	Continuous	Thermo 43i	HI CONC	MIDDLE	SOURCE MONITORING	SHUTDOWN	SU 1/1/1978 SD 3/29/2021
12-031-0098	Mandarin Rd	14932 Mandarin Rd, Jacksonville, FL 32223; 30.135869, -81.634094	SLAMS	PM _{2.5}	3	Continuous	Teledyne T640X	POP EXP	NBH	NEEDED BY REGULATION		SU 9/01/2019; FEM
			SLAMS	PM ₁₀	1	Continuous	Teledyne T640X	POP EXP	NBH	NEEDED BY REGULATION		SU 6/1/2019; FEM
12-031-0099	Sunny Acres	9429 Merrill Rd., Jacksonville, FL 32225; 30.354614, -81.547789	SLAMS	PM _{2.5}	1	Every 3rd Day	Thermo 2025i	POP EXP	NBH	NEEDED BY REGULATION	REPLACED BY FEM	SU 6/1/1999; Expected Replacement by FEM 10/2021
			SLAMS	PM _{2.5}	2	Every 12th Day	Thermo 2025i	POP EXP	NBH	QA COLLOCATION	SHUTDOWN	SU 6/1/1999; Collocated monitor; Expected SD 10/2021
			SLAMS	PM _{2.5}	3	Continuous	Teledyne T640	POP EXP	NBH	NEEDED BY REGULATION	ADD	SU 10/2021
			SLAMS	Ozone	1	Continuous	Thermo 49i	HI CONC	NBH	NEEDED BY REGULATION		SU 9/1/2002
12-031-0100	Mayo Clinic	13600 William Davis Pkwy, Jacksonville, FL 32224; 30.260420, -81.453341	SPM	PM _{2.5}	3	Continuous	Thermo 1405	POP EXP	URBAN	USED FOR AQI		SU 1/1/2004
12-031-0106	Cisco Drive	4770 Cisco Dr., Jacksonville, FL 32219; 30.378217, -81.840900	SPM	Ozone	1	Continuous	Thermo 49i	REGIONAL TRANSPORT	URBAN	USED FOR AQI		SU 9/28/2009
12-031-0108	Pepsi Place	5895 Pepsi Place, Jacksonville, FL 32319; 30.262730, -81.606826	SLAMS	CO	1	Continuous	Thermo 48i	SOURCE	MIDDLE	NEEDED BY REGULATION		SU 1/1/2014
			SLAMS	NO ₂	1	Continuous	Thermo 42i	SOURCE	MIDDLE	NEEDED BY REGULATION		SU 1/1/2014; Near-road Site
			SLAMS	PM _{2.5}	3	Continuous	Teledyne T640	HI CONC	MIDDLE	NEEDED BY REGULATION		SU 8/01/2019; FEM
Nassau County												
12-089-0005	Fernandina Beach Waste Water Treatment Plant (FBWWTP)	1007 S 5th St, Fernandina Beach, FL 32304; 30.658552, -81.463168	SLAMS	SO ₂	1	Continuous	Thermo 43i	HI CONC	NBH	NEEDED BY REGULATION		SU 1/1/1976
METROPOLITAN STATISTICAL AREA: ORLANDO - KISSIMMEE (LAKE, ORANGE, OSCEOLA AND SEMINOLE COUNTIES)												
Lake County												
AQS #	SITE NAME	ADDRESS/ COORDINATES	TYPE	POLLUTANT	POC	OPERATING SCHEDULE	SAMPLER	MONITORING OBJECTIVE	SPATIAL SCALE	STATEMENT OF PURPOSE	MODIFICATIONS	COMMENTS
12-069-0002	Clermont	1901 Johns Lake Rd., Clermont, FL 34711; 28.523889, -81.723333	SLAMS	Ozone	1	Continuous	Thermo 49i	POP EXP	NBH	MONITORING EXT COUNTY OF LARGE MET STAT AREA		SU 6/1/2000
Orange County												
12-095-0009	I-4 Near Road	525 S. Division Ave, Orlando, FL 32805; 28.534930, -81.384247	SLAMS	CO	1	Continuous	Thermo 48i	SOURCE	MIDDLE	NEEDED BY REGULATION		SU 7/1/2016; Near-road Site; Temporarily Closed
			SLAMS	NO ₂	1	Continuous	Thermo 42i	SOURCE	MIDDLE	NEEDED BY REGULATION		SU 7/1/2016; Near-road Site; Temporarily Closed
			SLAMS	PM _{2.5}	3	Continuous	Thermo 5014i	SOURCE	MIDDLE	NEEDED BY REGULATION		SU 2/1/2017; FEM; Near-road Site; Temporarily Closed
12-095-0010	Skyview Drive	7697 S. Orange Blossom Trail, Orlando, FL 32809; 28.453167, -81.397139	SLAMS	Ozone	1	Continuous	Thermo 49i	POP EXP	NBH	NEEDED BY REGULATION		SU 3/5/2020

12-095-2002	Lake Isle Estates - Winter Park	213 S. Denning Ave, Winter Park, FL 32789; 28.594950, -81.3638405	SPM	CO	1	Continuous	Thermo 48i	POP EXP	NBH	TRENDS MONITORING	RELOCATION	SU 3/23/1978; Relocation Expected: 10/2021		
			SLAMS	SO ₂	1	Continuous	Thermo 43i	HI CONC	NBH	FOR EFFECTIVENESS OF NEW REGULATIONS	RELOCATION	SU 1/1/1976; Relocation Expected: 10/2021		
			SLAMS	NO ₂	1	Continuous	Thermo 42i	POP EXP	URBAN	COMM-WIDE MONITORING	RELOCATION	SU 1/1/1981; Relocation Expected: 10/2021		
			SLAMS	Ozone	1	Continuous	Thermo 49i	HI CONC	NBH	NEEDED BY REGULATION	RELOCATION	SU 1/1/1976; Relocation Expected: 10/2021		
			SLAMS	PM ₁₀	1	Continuous	Thermo 5014i	POP EXP	NBH	NEEDED BY REGULATION	RELOCATION	SU 1/24/2015; Relocation Expected: 10/2021		
			SLAMS	PM _{2.5}	3	Continuous	Thermo 5014i	POP EXP	NBH	NEEDED BY REGULATION	RELOCATION	SU 10/1/2016; FEM; Relocation Expected: 10/2021		
			Osceola County											
12-097-2002	Osceola Co. Fire Station - Four Corners	8706 W Irlo Bronson Memorial Hwy (SR 192), Kissimmee, FL 34747; 28.347509, -81.636464	SLAMS	Ozone	1	Continuous	Thermo 49i	HI CONC	URBAN	URBAN SPRAWL		SU 9/1/1993		
Seminole County														
12-117-1002	Sanford	284-300 Broadmoor Rd., Lake Mary, FL 32773; 28.746111, -81.310556	SLAMS	Ozone	1	Continuous	Thermo 49i	HI CONC	URBAN	MONITORING EXT COUNTY OF LARGE MET STAT AREA		SU 1/1/1980		
			SLAMS	PM ₁₀	3	Continuous	Thermo 1405	POP EXP	NBH	NEEDED BY REGULATION		SU 12/22/2000		
			SLAMS	PM _{2.5}	1	Every 12th Day	Thermo 2025i	POP EXP	NBH	MONITORING EXT COUNTY OF LARGE MET STAT AREA		SU 1/7/1999; Collocated monitor		
			SLAMS	PM _{2.5}	4	Continuous	Teledyne T640	POP EXP	NBH	NEEDED BY REGULATION		SU 1/1/2018; FEM		
METROPOLITAN STATISTICAL AREA: SARASOTA - BRADENTON - VENICE (MANATEE AND SARASOTA COUNTIES)														
Manatee County														
AQS #	SITE NAME	ADDRESS/COORDINATES	TYPE	POLLUTANT	POC	OPERATING SCHEDULE	SAMPLER	MONITORING OBJECTIVE	SPATIAL SCALE	STATEMENT OF PURPOSE	MODIFICATIONS	COMMENTS		
12-081-3002	Port Manatee	1801 Piney Point Rd., Palmetto, FL 34221; 27.637890, -82.547480	SLAMS	Ozone	1	Continuous	2B Tech 202	HI CONC	NBH	NEEDED BY REGULATION		SU 4/1/1992; SD 5/31/2008; SU 6/10/2009		
12-081-4012	GT Bray Park	5502 33rd Ave Drive W., Bradenton, FL 34209; 27.475190	SPM	Ozone	1	Continuous	2B Tech 202	POP EXP	NBH	USED FOR AQI	REPLACE BY FEM	SU 2/1/1999; SD 5/31/2008; SU 6/10/2009		
12-081-4013	39th Street Park	5511 39th St. East, Bradenton, FL 34203; 27.442780, -82.513120	SPM	Ozone	1	Continuous	2B Tech 202	POP EXP	NBH	USED FOR AQI	ADD	SU 12/31/2020		
12-081-0028	Port Manatee DEP	1801 Piney Point Rd., Palmetto, FL 34221; 27.637890, -82.547480	SLAMS	SO ₂	1	Continuous	Thermo 43i	SOURCE	NBH	NEEDED BY REGULATION		SU 11/5/2013		
Sarasota County														
AQS #	SITE NAME	ADDRESS/COORDINATES	TYPE	POLLUTANT	POC	OPERATING SCHEDULE	SAMPLER	MONITORING OBJECTIVE	SPATIAL SCALE	STATEMENT OF PURPOSE	MODIFICATIONS	COMMENTS		
12-115-0013	Bee Ridge Park	4430 S. Lockwood Ridge Rd., Sarasota, FL 34231; 27.290556, -82.507222	SLAMS	PM _{2.5}	3	Continuous	Teledyne T640	POP EXP	NBH	NEEDED BY REGULATION		SU 1/1/2018; FEM		
12-115-1005	Lido Park	190 Taft Dr., Sarasota, FL 34236; 27.309995, -82.569689	SLAMS	Ozone	1	Continuous	Thermo 49i	HI CONC	URBAN	NEEDED BY REGULATION		SU 9/5/1989		
12-115-1006	Paw Park	4570 17th St., Sarasota, FL 34235; 27.350278, -82.479722	SLAMS	Ozone	1	Continuous	Thermo 49i	POP EXP	NBH	USED FOR AQI		SU 10/1/1999		
12-115-2002	Jackson Road	250 S. Jackson Rd., Venice, FL 34292; 27.089194, -82.362583	SLAMS	PM ₁₀	1	Continuous	Thermo 1405	POP EXP	NBH	NEEDED BY REGULATION		SU 9/19/2003; FEM		
			SPM	Ozone	1	Continuous	Thermo 1405	POP EXP	NBH	USED FOR AQI		SU 9/1/2003		
Lee County														
AQS #	SITE NAME	ADDRESS/COORDINATES	TYPE	POLLUTANT	POC	OPERATING SCHEDULE	SAMPLER	MONITORING OBJECTIVE	SPATIAL SCALE	STATEMENT OF PURPOSE	MODIFICATIONS	COMMENTS		
12-071-0005	Winkler Pump Station	1403 Princeton St., Ft. Myers, FL 33901; 26.602016, -81.877908	SLAMS	PM ₁₀	3	Continuous	Thermo 1405	POP EXP	NBH	NEEDED BY REGULATION	REPLACE BY FEM	SU 2/22/2001 REPLACEMENT EXPECTED 06/2021		
			SLAMS	PM _{2.5}	3	Continuous	Teledyne T640	POP EXP	NBH	NEEDED BY REGULATION	REPLACE BY FEM	SU 1/1/2018; REPLACEMENT EXPECTED 06/2021		
			SLAMS	PM _{2.5}	3	Continuous	Teledyne T640X	POP EXP	NBH	NEEDED BY REGULATION	ADD	SU EXPECTED 06/2021		
			SLAMS	PM ₁₀	3	Continuous	Teledyne T640X	POP EXP	NBH	NEEDED BY REGULATION	ADD	SU EXPECTED 06/2021		
			SLAMS	PM _{2.5}	4	Continuous	Teledyne T640X	POP EXP	NBH	QA COLLOCATION	ADD	Collocated monitor SU EXPECTED 06/2021		
			SLAMS	PM ₁₀	4	Continuous	Teledyne T640X	POP EXP	NBH	QA COLLOCATION	ADD	Collocated monitor SU EXPECTED 06/2021		
			SLAMS	Ozone	1	Continuous	49i	POP EXP	NBH	NEEDED BY REGULATION	ADD	SU EXPECTED 06/2021 Relocation from 12-071-3002		

Putnam County													
AQS #	SITE NAME	ADDRESS/ COORDINATES	TYPE	POLLUTANT	POC	OPERATING SCHEDULE	SAMPLER	MONITORING OBJECTIVE	SPATIAL SCALE	STATEMENT OF PURPOSE	MODIFICATIONS	COMMENTS	
12-107-1008	Palatka Barge Port	188 Comfort Rd., Palatka, FL 32177; 29.687748, -81.656509	SLAMS	SO ₂	1	Continuous	Thermo 43i	SOURCE	NBH	SOURCE MONITORING		SU 8/15/1991	
			SLAMS	PM ₁₀	3	Continuous	Thermo 1405	POP EXP/ SOURCE	NBH	SOURCE MONITORING		SU 12/13/2002	
MICROPOLITAN STATISTICAL AREA: LAKE CITY (COLUMBIA COUNTY)													
Columbia County													
AQS #	SITE NAME	ADDRESS/ COORDINATES	TYPE	POLLUTANT	POC	OPERATING SCHEDULE	SAMPLER	MONITORING OBJECTIVE	SPATIAL SCALE	STATEMENT OF PURPOSE	MODIFICATIONS	COMMENTS	
12-023-0002	Lake City - Veterans Domicile	751 SE Sycamore Terrace, Lake City, FL 32025; 30.178056, -82.619167	SLAMS	Ozone	1	Continuous	Thermo 49i	POP EXP	NBH	MONITOR IMPACT OF HIGH TRAFFIC		SU 11/1/2000	
			SPM	PM _{2.5}	3	Continuous	Thermo 1405	POP EXP	NBH	RURAL MONITORING		SU 5/17/2007	
MICROPOLITAN STATISTICAL AREA: HOMOSASSA SPRINGS (CITRUS COUNTY)													
Citrus County													
AQS #	SITE NAME	ADDRESS/ COORDINATES	TYPE	POLLUTANT	POC	OPERATING SCHEDULE	SAMPLER	MONITORING OBJECTIVE	SPATIAL SCALE	STATEMENT OF PURPOSE	MODIFICATIONS	COMMENTS	
12-017-0006	Crystal River Preserve	13450 W. Power Line Rd., Crystal River, FL 34428; 28.958644, -82.642965	SLAMS	SO ₂	1	Continuous	Thermo 43i	SOURCE	NBH	NEEDED BY REGULATION		SU 12/13/2013	
			SPM	PM _{2.5}	1	Continuous	Thermo 1405	POP EXP	NBH	RURAL MONITORING		SU 12/7/2015	
NOT IN A METROPOLITAN STATISTICAL AREA													
Holmes County													
AQS #	SITE NAME	ADDRESS/ COORDINATES	TYPE	POLLUTANT	POC	OPERATING SCHEDULE	SAMPLER	MONITORING OBJECTIVE	SPATIAL SCALE	STATEMENT OF PURPOSE	MODIFICATIONS	COMMENTS	
12-059-0004	Bonifay Tri-County Airport	1976 Tri County Airport Rd., Bonifay, FL 32425; 30.848611, -85.603889	SPM	Ozone	1	Continuous	Thermo 49i	POP EXP	REGIONAL	REGIONAL BACKGROUND		SU 9/1/1996	
			SPM	PM _{2.5}	3	Continuous	Thermo 1405	POP EXP	NBH	REGIONAL BACKGROUND		SU 6/14/2007	
Hamilton County													
12-047-0015	White Springs	Southeast CR 137, White Springs, FL 32096; 30.426363, -82.794841	SLAMS	SO ₂	1	Continuous	Thermo 43i	SOURCE	MIDDLE	SOURCE MONITORING		SU 9/18/1982	
			SPM	PM _{2.5}	3	Continuous	Thermo 1405	SOURCE	NBH	RURAL MONITORING		SU 5/17/2007	
IMPROVE NETWORK													
AQS #	SITE NAME	ADDRESS/ COORDINATES	TYPE	POLLUTANT	POC	OPERATING SCHEDULE	SAMPLER	MONITORING OBJECTIVE	SPATIAL SCALE	STATEMENT OF PURPOSE	MODIFICATIONS	COMMENTS	
12-129-0001	St. Marks Wildlife Refuge	County Rd. 59, St. Marks, FL 32355; 30.092500, -84.161111	SPM	PM _{2.5}		Every 3rd Day	IMPROVE	BKGD	URBAN	NEEDED BY REGULATION		SU 2000	
12-017-9000	Chassahowitzka National Wildlife Refuge	S Timbe Pines Ave., Homosassa, FL 34448; 28.7486, -82.5551	SPM	PM _{2.5}		Every 3rd Day	IMPROVE	TRANSPORT	URBAN	NEEDED BY REGULATION		SU 1993	
12-086-0030	Everglades National Park	Everglades National Park, FL	SPM	PM _{2.5}		Every 3rd Day	IMPROVE	BKGD	URBAN	NEEDED BY REGULATION		SU 1988	

List of Abbreviations:

AQI	Air Quality Index
BKGD	Background
CO	Carbon Monoxide
CSN	Chemical Speciation Network
EC/OC	Elemental Carbon/Organic Carbon
FRM	Federal Reference Method
GEN BKGD	General Background
HI CONC	High Concentration
MET	Implies that wind speed and wind direction instruments are on site
NAMS	National Air Monitoring Stations
NBH	Neighborhood
NCORE	National Core
NO ₂	Nitrogen Dioxide
NON-REG	Non-regulatory Monitoring
POP EXP	Population Exposure
PM _{2.5}	Particulate matter with aerodynamic diameter of 2.5 micro meter
PM ₁₀	Particulate matter with aerodynamic diameter of 10 micro meter
SLAMS	State and Local Air Monitoring Stations
SO ₂	Sulfur Dioxide
SPM	Special Purpose Monitors
SPEC. PM _{2.5}	Supplemental PM _{2.5} Speciation
SD	Shut Down
SU	Set Up
STN	Speciation Trends Network
UFP	Ultra Fine Particle
VOC	Volatile Organic Compound

APPENDIX D: AMBIENT AIR MONITORING INVENTORY

EPA requires an evaluation of the agency's ambient monitors and auxiliary support equipment. The condition of inventory should be categorized as "Good," "Fair" or "Poor," and indicate equipment, not in everyday use (e.g. spare or back-up). The ambient monitoring equipment inventories for Florida's monitoring agencies are provided below.

City of Jacksonville									
Property /Identification No.	Manufacturer and Model No.	Description	Location	Serial No.	Acquisition Date	Age	Initial Cost	Condition	Status
186859	N/A	Air Compressor	Lab	N/A	2009	12	1225.17	Fair	Backup
2002640	42i - Nox	Analyzer	Kooker Park	1170310010	N/A	N/A	N/A	Good	Active
2002645	42i - Nox	Analyzer	Pepsi Place	1170310009	N/A	N/A	N/A	Good	Active
188994	42i - Nox	Analyzer	Lab	0817630890	2010	11	11304.56	Fair	Backup
195337	42i - Nox	Analyzer	Lab	1327059041	N/A	N/A	N/A	Good	Parts
172824	43C - SO2	Analyzer	Lab	0421007303	N/A	N/A	N/A	Poor	Parts
175613	43C - SO2	Analyzer	Lab	0436610194	N/A	N/A	N/A	Fair	Parts
184697	43C - SO2	Analyzer	Lab	43C-75636-380	N/A	N/A	N/A	Fair	Parts
2002641	43i - SO2	Analyzer	Kooker Park	1170310008	N/A	N/A	N/A	Good	Active
180789	43i - SO2	Analyzer	Lab	611616471	2006	12	N/A	Good	Backup
176660	43i - SO2	Analyzer	Lab	0520811801	N/A	N/A	N/A	Fair	Backup
179549	43i - SO2	Analyzer	Lab	0600914730	N/A	N/A	N/A	Fair	Backup
193321	43i - SO2	Analyzer	Lab	1225154501	2012	9	10967.50	Poor	Parts
197214	43i - SO2	Analyzer	Lab	1436363426	2014	7	12457.00	Good	Backup
2002637	43i - SO2	Analyzer	Lab	1170310006	N/A	N/A	N/A	Good	Active
N/A	43i-SO2	Analyzer	Cedar Bay	1170310007	N/A	N/A	N/A	Good	Inactive
167934	48C - CO	Analyzer	Lab	48C-67479-356	N/A	N/A	N/A	Good	Backup
167932	48C - CO	Analyzer	Lab	48C-67941-356	N/A	N/A	N/A	Fair	Parts
167935	48C - CO	Analyzer	Lab	48C-67941-359	2001	20	8559.00	Poor	Parts
N/A	48C - CO trace	Analyzer	Lab	48CTL-67186-356	N/A	N/A	N/A	Fair	Parts
195338	48i - CO	Analyzer	Pepsi Place	1308857434	2014	7	12467.00	Good	Active
180679	48i - CO	Analyzer	Lab	0611616470	N/A	N/A	N/A	Fair	Parts
193160	48i - CO	Analyzer	Lab	1216753230	N/A	N/A	N/A	Fair	Parts
197215	48i - CO	Analyzer	Lab	1436363425	2014	7	12467.00	Poor	Backup
199824	48i - CO	Analyzer	Lab	1160600006	2016	5	12785.75	Good	Backup
2002638	48i - CO	Analyzer	Lab	1170310013	N/A	N/A	N/A	Good	Inactive
N/A	48i - CO	Analyzer	Lab	1170310014	N/A	N/A	N/A	Good	Inactive
174139	49C - O3	Analyzer	Lab	423707710	2004	17	6354.00	Fair	Parts
174138	49C - O3	Analyzer	Lab	0423707712	2004	17	6354.00	Fair	Parts
174133	49C - PS	Analyzer	Lab	0423707707	2004	17	8127.00	Fair	Parts
N/A	49i - ozone	Analyzer	Lab	1170480025	N/A	N/A	N/A	Good	Active
2002639	49i - ozone	Analyzer	Mayo	117310016	N/A	N/A	8702.90	Good	Active
197158	49i - ozone	Analyzer	Cisco Dr	1430863374	2015	6	9640.00	Good	Active
180678	49i - ozone	Analyzer	Sheffield Elementary	0611616471	N/A	N/A	N/A	Good	Active
186855	49i - ozone	Analyzer	Lab	CM09040077	2009	12	6978.40	Fair	Backup
186856	49i - ozone	Analyzer	Lab	CM09040078	2009	12	6978.40	Fair	Parts
186857	49i - P5 ozone	Analyzer	Sheffield Elementary	0908935367	2009	12	9416.00	Good	Active
186858	49i - PS ozone	Analyzer	Mayo	1170480025	N/A	N/A	N/A	Good	Active
N/A	49i - PS ozone	Analyzer	Cisco Dr	0908935366	2009	12	9416.00	Good	Active
N/A	49i - PS ozone	Analyzer	Lab	1430863375	2015	6	N/A	Good	Active
138481	49i - P5 ozone	Analyzer	Lab	1225154500	2012	6	11233.50	Fair	Backup
106278	N/A	Balance	Lab	3411155	N/A	N/A	N/A	Poor	Obsolete
195340	6100	Calibrator	Lab	5736	2008	13	N/A	Good	Active
189416	6100	Calibrator	Lab	4776	2010	11	8775.00	Good	Active
182786	6100	Calibrator	Pepsi Place	3887	N/A	N/A	N/A	Fair	Backup
184538	6100	Calibrator	Lab	4306	N/A	N/A	N/A	Fair	Active
189417	6100	Calibrator	Lab	4775	2010	11	8775.00	Fair	Backup
197600	6100	Calibrator	Cedar Bay	6508	2015	6	8887.50	Fair	Backup
182787	6100	Calibrator	Kooker Park	3886	N/A	N/A	N/A	Fair	Backup
189416	6100	Calibrator	Lab	4776	2010	11	8775.00	Good	Backup
2002229	6100	Calibrator	Pepsi Place	7585	2017	4	N/A	Good	Backup
184536	6100	Calibrator	Lab	4312	N/A	N/A	N/A	Fair	Backup
197599	6100	Calibrator	Lab	6509	2015	6	8887.50	Fair	Backup
2002228	6100	Calibrator	Pepsi Place	7586	2017	4	N/A	Good	Active
2002230	6100	Calibrator	Roselle & Copeland	7584	2017	4	N/A	Good	Backup
187085	6100	Calibrator	Kooker Park	4491	2009	12	8775.00	Good	Active
187084	6100	Calibrator	Lab	4490	2009	12	8775.00	Good	Backup
172646	Computer	Computer	Kooker Park	KCBX2R7	N/A	N/A	N/A	Fair	Active
172648	Computer	Computer	Mayo	KCTA57T	N/A	N/A	N/A	Fair	Active
N/A	Computer	Computer	Ft. Caroline	4VGTVN1	N/A	N/A	N/A	Fair	Inactive
167681	Computer - Dell 1400	Computer	Cubicle	N/A	N/A	N/A	N/A	Fair	Active
184695	Computer - Dell Latitude D630	Computer	Pepsi Place	BPVYZF1	N/A	N/A	N/A	Fair	Active
N/A	Computer - Dell OptiPlex	Computer	Cisco Dr	79NP1B1	N/A	N/A	N/A	Fair	Active
172512	Computer - IBM	Computer	Cedar Bay	KCRZ00A	N/A	N/A	N/A	Fair	Active
180783	Computer - Think Centre	Computer	Cubicle	LKKL5G	N/A	N/A	N/A	Fair	Active
172575	Computer IBM	Computer	Lab	KCRR74F	N/A	N/A	N/A	Fair	Active
N/A	Laptop - ThinkPad (Alvin)	Computer	Cubicle	R9-EBZK1	N/A	N/A	N/A	Fair	Active
184695	Laptop - ThinkPad PPL	Computer	Pepsi Place	BPVYZF1	N/A	N/A	N/A	Fair	Active
172513	Computer	Computer	Sheffield Elementary	KCRR91M	N/A	N/A	N/A	Fair	Active
162147	Computer - Dell XPS R400	Computer	Cubicle	GDKR0	N/A	N/A	N/A	Fair	Active
183820	8832	Data Logger	Lab	A1943	2004	17	N/A	Good	Inactive
172529	8832	Data Logger	Transferred to Broward County from lab	A0541	2004	17	N/A	Good	Inactive
N/A	8832	Data Logger	Lab	A0538	2004	17	N/A	Good	Inactive
171778	8832	Data Logger	Lab	A0543	2004	17	N/A	Good	Inactive
183819	8832	Data Logger	Lab	A1942	2004	17	N/A	Good	Inactive
172525	8832	Data Logger	Lab	A0547	2004	17	N/A	Good	Inactive
195341	8832	Data Logger	Lab	A4688K	2014	7	N/A	Good	Inactive
172516	8832	Data Logger	Lab	A0540	N/A	N/A	N/A	Fair	Parts
N/A	8832	Data Logger	Lab	A0542	N/A	N/A	N/A	Fair	Backup
172526	8832	Data Logger	Lab	A0544	N/A	N/A	N/A	Fair	Parts
172517	8832	Data Logger	Lab	A0545	N/A	N/A	N/A	Fair	Backup
172518	8832	Data Logger	Lab	A0546	N/A	N/A	N/A	Fair	Good

172528	8832	Data Logger	Transferred to Broward County from lab	A0549	N/A	N/A	N/A	Fair	Good
172527	8832	Data Logger	Transferred to Broward County from lab	A0548	N/A	N/A	N/A	Fair	Inactive
172524	8832	Data Logger	Transferred to Broward County from lab	A0587	N/A	N/A	N/A	Fair	Backup
189681	8832	Data Logger	Lab	A3937K	2004	17	N/A	Good	Inactive
189680	8832	Data Logger	Lab	A3936K	N/A	N/A	N/A	Good	Inactive
172522	8832	Data Logger	Lab	A0586	N/A	N/A	N/A	Good	Inactive
2007832	8872	Data Logger	Kooker Park	8872_0842	2018	3	7911.22	Good	Active
2007839	8872	Data Logger	Sheffield Elementry	8872_0850	2018	3	7911.22	Good	Active
2007838	8872	Data Logger	Cedar Bay	8872_0847	2018	3	7911.22	Good	Active
2007834	8872	Data Logger	Mandarin Rd	8872_0851	2018	3	7911.22	Good	Active
2007831	8872	Data Logger	Mayo	8872_0846	2018	3	7911.22	Good	Active
2007836	8872	Data Logger	Cisco Dr	8872_0849	2018	3	7911.22	Good	Active
2007833	8872	Data Logger	Pepsi Place	8872_0844	2018	3	7911.22	Good	Active
2007835	8872	Data Logger	Lab	8872_0848	2018	3	7911.22	Good	Backup
2007837	8872	Data Logger	Lab	8872_0845	2018	3	7911.22	Good	Backup
171778	Enclosure	Enclosure	Mandarin Rd	343G-10 (CO# from inven)	N/A	N/A	N/A	Fair	Inactive
184118	Definer 220 H	flow standard	Lab	112786	N/A	N/A	N/A	Good	Backup
162935	Manometer	Manometer	Lab	11MNO2	N/A	N/A	N/A	Fair	Backup
195344	Met Sensor	Met Sensor	Pepsi Place	N/A	N/A	N/A	N/A	Fair	Active
195347	Met Tower	Met Tower	Pepsi Place	N/A	N/A	N/A	N/A	Fair	Active
N/A	ThinkVision Monitor	Monitor	Kooker Park	8894881	N/A	N/A	N/A	Fair	Backup
125742	Toxgard - CO Monitor	Monitor	Lab	N/A	N/A	N/A	N/A	Fair	Active
144535	Toxgard - CO Monitor	Monitor	Lab	N/A	N/A	N/A	N/A	Fair	Active
144537	Toxgard - CO Monitor	Monitor	Lab	N/A	N/A	N/A	N/A	Fair	Active
144536	Toxgard - CO Monitor	Monitor	Roselle & Copeland	N/A	N/A	N/A	N/A	Fair	Inactive
189418	O3 PS - 6103	O3 PS - 6103	Lab	4781	N/A	N/A	N/A	Fair	Backup
105038	Olfactometer	Olfactometer	File Room	N/A	N/A	N/A	N/A	Poor	Backup
105039	Olfactometer	Olfactometer	File Room	N/A	N/A	N/A	N/A	Poor	Backup
N/A	Opti Plex 780	Opti Plex 780	Lab	CCFVN1	N/A	N/A	N/A	Fair	Active
167292	HP Laser Jet 2100	Printer	Lab	USGZ182467	N/A	N/A	N/A	Fair	Backup
164189	HP Laser Jet 2101	Printer	Lab	N/A	N/A	N/A	N/A	Fair	Backup
177084	HP Laser Jet 2430dn	Printer	Cubicle	N/A	N/A	N/A	N/A	Fair	Backup
195345	Computer Rack	Rack	Pepsi Place	N/A	N/A	N/A	N/A	Good	Active
195346	Computer Rack	Rack	Pepsi Place	N/A	N/A	N/A	N/A	Good	Active
183596	2025	Sampler	Lab	2025B219720706	N/A	N/A	N/A	Fair	Backup
197212	2025i	Sampler	Lab	2025i206831409	2014	7	16361.25	Good	Inactive
197213	2025i dup	Sampler	Sunny Acres	2025i206911409	2014	7	16361.25	Good	Backup
197211	2025i	Sampler	Sunny Acres	2025i206891409	2014	7	16361.25	Good	Active
197694	2025i	Sampler	Lab	2025iW207931504	2015	6	17050.77	Good	Active
197615	5014i	Sampler	Pepsi Place	CM14501004	2015	6	16880.00	Good	Inactive
195339	5014i	Sampler	Lab	CM13351001	2014	7	15213.66	Fair	Backup
N/A	TE 1400A	Sampler	Lab	140AB267240705	N/A	N/A	N/A	Fair	Parts
188469	TE 1400ab	Sampler	Lab	140AB275771001	N/A	N/A	N/A	Fair	Parts
N/A	TE rp 1400A	Sampler	Lab	140AB267570706	N/A	N/A	N/A	Fair	Parts
171776	TEOM 1400	Sampler	Lab	140AB245080303	N/A	N/A	N/A	Fair	Parts
171777	TEOM 1400AB	Sampler	Lab	140AB245050303	N/A	N/A	N/A	Good	Inactive
197614	TEOM 1405	Sampler	Sheffield Elementry	1405A230661501	2015	6	17075.00	Good	Active
199821	TEOM 1405	Sampler	Mayo	1405A235821603	2016	5	16890.13	Good	Active
197613	TEOM 1405	Sampler	Lab	1405A230821502	2015	6	17075.00	Good	Inactive
N/A	Thermo 1405	Sampler	Lab	1405A241581808	N/A	N/A	N/A	Good	Backup
199822	TEOM 1405	Sampler PM10	Kooker Park	1405A235831603	2016	5	16890.13	Good	Active
199823	TEOM 1405	Sampler PM2.5	Kooker Park	1405A236021603	2016	5	16890.13	Good	Active
N/A	CAS Cargo Container	Shelter	Kooker Park	N/A	2018	3	85852.38	Good	Active
171440	Sonic Anemometer	Sonic Anemometer	Lab	N/A	N/A	N/A	N/A	Poor	Parts
171441	Sonic Anemometer	Sonic Anemometer	Lab	N/A	N/A	N/A	N/A	Poor	Parts
171442	Sonic Anemometer	Sonic Anemometer	Lab	N/A	N/A	N/A	N/A	Poor	Parts
116737	Supply Cabinet - metal	Supply Cabinet - metal	Lab	N/A	N/A	N/A	N/A	Fair	Active
2010486	Teledyne	T640	Pepsi Place	681	2019	2	23987.00	Good	Active
N/A	Teledyne	T640X	Mandarin Rd	725	2019	2	37194.00	Good	Active
168912	Trailer	Trailer	Sheffield Elementry	N/A	N/A	N/A	N/A	Poor	Active
144808	Trailer	Trailer	Cedar Bay	N/A	1994	27	4643.20	Poor	Active
N/A	Trailer	Trailer	Mandarin Rd	N/A	N/A	N/A	N/A	Poor	Active
153455	Trailer	Trailer	Mayo	N/A	N/A	N/A	N/A	Poor	Active
184190	Trailer	Trailer	Cisco Dr	N/A	2009	12	5191.10	Good	Active
195343	Trailer	Trailer	Pepsi Place	N/A	N/A	N/A	N/A	Good	Active
138480	Trailer	Trailer	Lab	N/A	1991	30	3697.90	Poor	Active
175935	Trailer	Trailer	Roselle & Copeland	N/A	2005	16	5755.00	Poor	Inactive
153454	Trailer	Trailer	Ft. Caroline	N/A	N/A	N/A	N/A	Poor	Inactive
65951	Dial-A-Volt	voltage supplyf	Lab	802	N/A	N/A	N/A	Good	Active
N/A	Dial-A-Volt	voltage supplyf	Lab	801	N/A	N/A	N/A	Good	Active
186648	111	Zero Air Gen	Lab	907935555	2009	12	3334.17	Good	Active
195342	701H	Zero Air Gen	Pepsi Place	753	2014	7	7672.32	Good	Active
186647	TE 111	Zero Air Gen	Sheffield Elementry	907935554	2009	12	3334.17	Good	Active
2005522	Teledyne 701	Zero Air Gen	Kooker Park	5931	N/A	N/A	4756.75	Good	Active
2005521	Teledyne 701	Zero Air Gen	Lab	5933	N/A	N/A	4756.75	Good	Backup
2005523	Teledyne 701	Zero Air Gen	Lab	5930	N/A	N/A	4756.75	Good	Backup
2005524	Teledyne 701	Zero Air Gen	Lab	5932	N/A	N/A	4756.75	Good	Backup
2002358	Teledyne 701	Zero Air Gen	Lab	5975	2017	4	5236.22	Good	Backup
2002360	Teledyne 701	Zero Air Gen	Lab	5874	2017	4	5236.22	Good	Backup
2002357	Teledyne 701	Zero Air Gen	Lab	5876	2017	4	5236.22	Good	Backup
2002359	Teledyne 701	Zero Air Gen	Cedar Bay	5877	2017	4	5236.22	Good	Active

Inventory Report

Property Inventory

Report Created: 05/12/2021 16:26

As of: 05/12/2021

Property No.	Description	Location	Acquisition Date	Age	Initial Cost	Serial Number	Condition	Status
107234	Opsis AR-500 AR500-E-665 Chinook Engineering Streamline FTS	Weigh Lab Room B107	5/8/2000	21	\$163,950	AR500-E-665	Good	Active
107471	MRAS-4	Standards Lab Room B105 Cab A	6/1/2000	20	\$1,120	MRAS-4	Good	Active
108298	Opsis 500 OC500-1-029	Standards Lab Room B105	8/1/2000	20	\$19,150	OC500-1-029	Good	Active
87449	Dasibi 5008 207	Trailer Dep 3658			\$13,350		207	Good
88409	Wells Cargo 1WC200J1153030266	B0030002	12/12/1994	26	\$9,074.93	1WC200J1153030266	Good	Active
89695	Aluma Tower n/a	A0590004	10/20/1994	26	\$1,300	n/a	Good	Active
89696	Aluma Tower n/a	B0030002	10/20/1994	26	\$1,300	n/a	Good	Active
89803	Bios DC-2 B0254	OAM QA Room B105	12/17/1994	26	\$3,185.73	B0254	Good	Active
89804	Bios DC-2 B0252	Trailer Dep 3658	12/17/1994	26	\$3,185.74	B0252	Good	Marked for Surplus
90534	Dell 2Q70C	E0150002	2/6/1995	26	\$3,455	2Q70C	Good	Active
91944	Wells Cargo Gas Cylinder Rack n/a	Trailer Dep 3658	12/6/1995	25	\$1,150	n/a	Good	Active
91947	Wells Cargo Gas Cylinder Rack n/a	Trailer Dep 3658	12/6/1995	25	\$1,450	n/a	Good	Active
92727	Wells Cargo 1WC200D1953033346	MRAS Shop Parking Lot	10/2/1995	25	\$6,543.22	1WC200D1953033346	Good	Active
93875	Bios DC-2 B399	MRAS Shop D101A	12/26/1995	25	\$2,470	B399	Good	Active
93878	Bios DC-2 B404	Trailer Dep 3658	12/26/1995	25	\$2,470	B404	Good	Active
96282	Mettler 1115282625	Standards Lab Room B105	4/1/1997	24	\$9,608.75		1115282625	Good
99069	Bios DC-2 B-678	Trailer Dep 3658	2/3/1998	23	\$3,638.89	B-678	Good	Marked for Surplus
99070	Bios DC-2 B680	Trailer Dep 3658	2/3/1998	23	\$3,638.88	B680	Good	Marked for Surplus
EP004132	Wells Cargo 1WC200J11W3039118	G0730012	3/25/1998	23	\$9,930	1WC200J11W3039118	Good	Active
100505	Aluma Tower n/a	E0712002	11/19/1997	23	\$1,617.35	n/a	Good	Active
100506	Aluma Tower n/a	G0730012	11/19/1997	23	\$1,617.36	n/a	Good	Active
EP004606	Wells Cargo 1WC200J12X3042742	B0890005	11/10/1999	21	\$7,660	1WC200J12X3042742	Good	Active
	Wells Cargo EW2011							
EP004608	1WC200J14X3042743	B0470015	11/10/1999	21	\$7,660	1WC200J14X3042743	Good	Active
	Chinook Engineering FTS 57-004506-							
105200	00001	Duval County	12/14/1999	21	\$1,095	57-004506-00001	Good	Active
105948	Sony Mavica 123035	OAM QA Room B105	11/10/1999	21	\$903.95		123035	Good
	Thermo Environmental Instruments, Inc							
106222	42C 3860-636	Palm Beach County	12/14/1999	21	\$8,489	3860-636	Good	Active
106635	Aluma Tower Met Tower n/a	B0470015	1/28/2000	21	\$1,590	n/a	Good	Active
106636	Aluma Tower n/a	B0890005	1/28/2000	21	\$1,590	n/a	Good	Active
106637	Aluma Tower n/a	A0910002	1/28/2000	21	\$1,590	n/a	Good	Active
106638	Aluma Tower AT91204-L1-1	C0830004	1/28/2000	21	\$1,590	AT91204-L1-1	Good	Active
106639	Aluma Tower AT91204-4-8	MRAS Shop Parking Lot	1/28/2000	21	\$1,590	AT91204-4-8	Good	Active
106640	Aluma Tower n/a	B0230002	1/28/2000	21	\$1,590	n/a	Good	Active
106642	Aluma Tower AT91204-L1-#9	A0050006	1/28/2000	21	\$1,590	AT91204-L1-#9	Good	Active
106643	Aluma Tower T-135 n/a	A1130015	1/28/2000	21	\$1,590	n/a	Good	Active
106672	R&P 1400AB 140AB227819911	Trailer Dep 3658	1/13/2000	21	\$18,961.69	140AB227819911	Good	Active
106674	R&P 1400AB 140AB227859911	Trailer Dep 3658	1/13/2000	21	\$18,961.69	140AB227859911	Good	Marked for Surplus
106634	Aluma Tower AT91204-L1-4	C0690002	1/28/2000	21	\$1,590	AT91204-L1-4	Good	Active
	Wells Cargo EW2011							
EP003785	1WC200J18T3034008	Dumpster	6/21/1996	24	\$9,381	1WC200J18T3034008	Good	Active
30277	Wells Cargo 1WC200J19M3022127	C0094001	10/2/1991	29	\$9,020	1WC200J19M3022127	Good	Active
31034	Aluma Tower AT4794-C-11-8	BMC Fenced Lot	11/21/1991	29	\$1,148	AT4794-C-11-8	Good	Active
90594	Wells Cargo 1WC200J10R3029641	C1275002	1/10/1995	26	\$9,500	1WC200J10R3029641	Good	Active
26441	Aluma Tower n/a	C1275002	10/16/1987	33	\$1,100	n/a	Good	Active
	Wells Cargo EW2011							
89717	1WC200J16R3028877	C1171002	8/15/1994	26	\$9,074.93	1WC200J16R3028877	Good	Active
93281	Aluma Tower T-135 n/a	E0713002	9/1/1995	25	\$1,388	n/a	Good	Active
89330	Wells Cargo n/a	F1110013	9/1/1994	26	\$9,500	n/a	Good	Active
115507	R&P 1400AB 140AB245470304	Trailer Dep 3658	5/13/2003	17	\$17,460	140AB245470304	Good	Marked for Surplus
115508	R&P 1400A 140AB245490304	Trailer Dep 3658	5/13/2003	17	\$17,460	140AB245490304	Good	Marked for Surplus
111717	Opsis 150MM Cell n/a	OAM QA Room B105	5/10/2002	19	\$3,600	n/a	Good	Active
111718	Opsis 110 mm Cell n/a	OAM QA Room B105	5/10/2002	19	\$2,600	n/a	Good	Active
111719	Opsis n/a	Hillsborough County	5/10/2002	19	\$12,950	n/a	Good	Active
111720	Opsis OC500 n/a	OAM QA Room B105	5/10/2002	19	\$12,950	n/a	Good	Active
111721	Opsis Optical Bench n/a	MRAS Shop D101	5/10/2002	19	\$21,870	n/a	Good	Active
109218	R&P 1400AB 140AB234100012	Trailer Dep 3658	3/20/2001	20	\$16,975	140AB234100012	Good	Marked for Surplus
109220	R&P 1400AB 140AB233280011	LabAC-17	3/20/2001	20	\$16,975	140AB233280011	Good	Marked for Surplus
109632		548717 Standards Lab Room B105	3/22/2001	20	\$1,190		548717	Good
109633		535908 Standards Lab Room B105	3/22/2001	20	\$1,190		535908	Good
109634		535888 Standards Lab Room B105	3/22/2001	20	\$1,190		535888	Good
109635	LF-1	Standards Lab Room B105	3/21/2001	20	\$1,120	LF-1	Good	Active
109636	Chinook Engineering LF-2	OAM QA Room B105	3/21/2001	20	\$1,120	LF-2	Good	Active
109637	LF-3	Standards Lab Room B105	3/21/2001	20	\$1,120	LF-3	Good	Active
109638	LF-4	OAM QA Room B105	3/21/2001	20	\$1,120	LF-4	Good	Active
109727	EKTO 3200-13A	Trailer DNR 2096	3/20/2001	20	\$4,795	3200-13A	Good	In Storage
109912		120524 B416	4/3/2001	20	\$2,225		120524	Good
110689	Aluma Tower n/a	E0550003	8/27/2001	19	\$1,660	n/a	Good	Active
999999	Aluma Tower n/a	Budget Storage Warehouse	8/27/2001	19	\$1,660	n/a	Good	In Storage
110690	Aluma Tower n/a	LabA137A	8/27/2001	19	\$1,660	n/a	Good	Active
110946	R&P 1400AB 140AB235430103	Trailer Dep 3658	5/8/2001	20	\$16,975	140AB235430103	Good	Marked for Surplus
111336	Adam 5000 IAA0104612	Weigh Lab Room B107	12/7/2001	19	\$1,300	IAA0104612	Good	Marked for Surplus
111487	R&P 1400AB 140AB238020110	Trailer Dep 3658	11/13/2001	19	\$16,995	140AB238020110	Good	Marked for Surplus
112109	R&P 1400AB 140AB239110201	Trailer Dep 3658	2/7/2002	19	\$17,460	140AB239110201	Good	Active
	Wells Cargo EW2011							
EP004828	1WC200J17Y3043550	E0210004	5/15/2000	2				

EP004831	Wells Cargo EW2011 1WC200J19Y3043551	A0910002	5/2/2000	21	\$10,188 1WC200J19Y3043551	Good	Active
EP004832	Wells Cargo 1WC200J14Y3043554	A0050006	5/2/2000	21	\$10,188 1WC200J14Y3043554	Good	Active
	Wells Cargo EW2011						
EP004834	1WC200J10Y3043549	D1010005	4/17/2000	21	\$10,188 1WC200J10Y3043549	Good	Active
EP004844	Wells Cargo EW2011 NEED VIN #	A1130015	6/12/2000	20	\$10,188 NEED VIN #	Good	Active
EP004845	Wells Cargo	E0550003	6/26/2000	20	\$10,188	Good	Active
	Wells Cargo EW2011						
BL605015	1WC200J18Y3043556	C0090007	7/10/2000	20	\$10,188 1WC200J18Y3043556	Good	Active
BL605016	Wells Cargo 04913	C0830004	7/31/2000	20	\$10,188 4913	Good	Active
	Wells Cargo EW2011						
BL605017	1WC200J16Y3043555	C0090011	10/2/2000	20	\$10,188 1WC200J16Y3043555	Good	Active
EP004955	Wells Cargo 1WC200J19S3043730	B1071008	10/4/2000	20	\$9,094 1WC200J19S3043730	Good	Active
EP003904	Ford Expedition 1FMEU17L2VLB74797	BMC Motor Pool	5/28/1997	23	\$25,483 1FMEU17L2VLB74797	Good	Active
EP006105	Toyota Prius JTDKB20U953054887	BMC Motor Pool			\$0 JTDKB20U953054887	Good	Active
EP004535	Ford Expedition 1FMRU17L3XLB52263	OAM QA Bruce Ferrier	5/3/1999	22	\$24,819 1FMRU17L3XLB52263	Good	Active
ER015197	Locally Made T# DNR-2096	BMC Parking Lot	6/30/1980	40	\$2,000 T# DNR-2096	Good	Active
ERO17411	Hastings Mass Flow Meter 0-13344	Standards Lab Room B105	5/31/1983	37	\$1,281.35 0-13344	Good	Active
ERO20029	Dasibi 1009 133	OAM QA Room B105			\$6,900 133	Good	Active
ERO22570	KB22-2	Trailer Dep 3658			\$5,860 KB22-2	Good	In Storage
ERO27859	Hewlett Packard 2304A47503	OAM Offices	3/6/1989	32	\$810 2304A47503	Good	Lost/Missing/Stolen
ERO29230	Hastings 400 168	Standards Lab Room B105 Cab D			\$3,187.66 168	Good	In Storage
	Thermo Environmental Instruments, Inc						
ERO30204	49 49-34655-248	LabAC-17 Shelf B	9/3/1991	29	\$6,174 49-34655-248	Good	Lost/Missing/Stolen
ERO31035	Aluma Tower T-135 n/a	E0210004	11/21/1991	29	\$1,148 n/a	Good	Active
ERO32844	13142/18003	Trailer Dep 3658			\$1,723.46 13142/18003	Good	Marked for Surplus
EP005580	Wells Cargo 1WC200J2223047926	A0590004	1/17/2002	19	\$10,812 1WC200J2223047926	Good	Active
	Hastings Mass Flow Controller						
113829	AW02313002	Standards Lab Room B105	7/26/2002	18	\$1,629 AW02313002	Good	Active
106801	Bios DC-2 B936	MRAS Shop D101	1/10/2000	21	\$3,261 B936	Good	Active
106605	Bios DC-2M B 1241	Standards Lab Room B105	7/31/2002	18	\$3,147.25 B 1241	Good	Active
106606	Bios DC-2 B 1242	Standards Lab Room B105	8/21/2002	18	\$3,147.25 B 1242	Good	Active
105740	Environics 6103 2910	Trailer Dep 3658	10/31/2002	18	\$11,310.30 2910	Good	Marked for Surplus
89802	Bios DC-2 B0255	Trailer Dep 3658	12/17/1994	26	\$3,185.73 B0255	Good	Marked for Surplus
93883	Wells Cargo 1WC200J16T3034007	B0013012	6/21/1996	24	\$9,381 1WC200J16T3034007	Good	Active
93280	Aluma Tower n/a	B0013012	9/1/1995	25	\$1,388 n/a	Good	Active
114162	R&P 1400A 140AB242930209	Trailer Dep 3658	12/25/2003	17	\$16,995 140AB242930209	Good	Marked for Surplus
	Dwyer Instruments Incline Manometer						
21179	400-10	MRAS Shop D101	3/15/1985	36	\$500 400-10	Good	Active
EP005160	Dodge 2500 1B7KC23W71J589281	MRAS Shop D101	4/30/2001	20	\$20,198 1B7KC23W71J589281	Good	Active
108916	BGI Incorporated TriCal 65	Standards Lab Room B105	12/12/2002	18	\$2,028 65	Good	Active
108995	BGI Incorporated TriCal 66	Nature Coast	12/11/2002	18	\$2,028 66	Good	Active
108997	BGI Incorporated TriCal 67	First Coast	12/11/2002	18	\$2,028 67	Good	Active
109126	BGI Incorporated TriCal 68	Lee Island Coast	12/11/2002	18	\$2,028 68	Good	Active
	Wells Cargo WC200E						
EP005299	1WC200E1733049495	BMC Fenced Lot	2/18/2003	18	\$10,277 1WC200E1733049495	Good	Active
114706	Environics 6103 3046	Trailer Dep 3658	2/19/2003	18	\$11,310.30 3046	Good	Marked for Surplus
114707	Environics 6103 3062	LabA137I	2/19/2003	18	\$11,310.30 3062	Good	Marked for Surplus
93279	Aluma Tower n/a	A0330004	9/1/1995	25	\$1,388 n/a	Good	Active
115096	Environics 3103 3064	Trailer Dep 3658	3/27/2003	18	\$0 3064	Good	Marked for Surplus
106644	Aluma Tower AT9120405-6	D1010005	1/28/2000	21	\$1,590 AT9120405-6	Good	Active
ER030281	Wells Cargo EW2011WC22131S	D1056006	10/2/1991	29	\$9,020 EW2011WC22131S	Good	Active
EPA Supplied	R&P Partisol 2025 2025A205639807	Trailer DNR 2096	9/1/1998	22	\$0 2025A205639807	Good	Marked for Surplus
ER031217	Wells Cargo 1WC200J12N3022729	D1056005	1/31/1992	29	\$8,991.03 1WC200J12N3022729	Good	Active
	Wells Cargo EW2011						
30279	1WC200J12M3022129	E0710005	10/2/1991	29	\$9,020 1WC200J12M3022129	Good	Active
30136	Aluma Tower T-135-35 n/a	MRAS Shop D101	11/21/1991	29	\$1,148 n/a	Good	Marked for Surplus
	Thermo Environmental Instruments, Inc						
26880	43A 43A-22800-207	D1052006	1/1/1989	32	\$8,000 43A-22800-207	Good	Active
88410	Wells Cargo 1WC200J14R3028876	D1050010	9/23/1994	26	\$0 1WC200J14R3028876	Good	Active
ER031037	Aluma Tower n/a	D1012001	11/21/1991	29	\$1,148 n/a	Good	Active
31305	Wells Cargo 1WC200JIXN302977	C0830003	11/21/1991	29	\$9,020 1WC200JIXN302977	Good	Active
100507	Aluma Tower AT71198-102-3	C0830003	11/19/1997	23	\$1,617.35 AT71198-102-3	Good	Active
120171	Chinook Engineering FTS HL1	Standards Lab Room B105 Cab I	4/21/2004	17	\$1,835 HL1	Good	Active
120172	Chinook Engineering FTS HL2	Standards Lab Room B105 Cab I	4/21/2004	17	\$1,835 HL2	Good	Active
119262	ESC 8832 A0451	Weigh Lab Room B107	8/12/2004	16	\$6,270 A0451	Good	Marked for Surplus
119263	ESC 8832 A0457	Trailer Dep 3658	2/24/2004	17	\$6,270 A0457	Good	Marked for Surplus
119264	ESC 8832 A0458	MRAS Shop D101	8/12/2004	16	\$6,270 A0458	Good	Marked for Surplus
119265	ESC 8832 A0463	Weigh Lab Room B107	2/20/2004	17	\$7,220 A0463	Good	Marked for Surplus
119266	ESC 8832 A0464	Trailer Dep 3658	2/20/2004	17	\$7,220 A0464	Good	Marked for Surplus
119267	ESC 8832 A0465	Trailer Dep 3658	8/12/2004	16	\$6,270 A0465	Good	Marked for Surplus
119269	ESC 8832 A0467	Trailer Dep 3658	8/12/2004	16	\$6,270 A0467	Good	Marked for Surplus
119270	ESC 8832 A0473	Trailer Dep 3658	2/24/2004	17	\$6,270 A0473	Good	Marked for Surplus
119271	ESC 8832 A0487	Trailer Dep 3658	3/1/2004	17	\$6,270 A0487	Good	Marked for Surplus
119272	ESC 8832 A0488	Weigh Lab Room B107	3/1/2004	17	\$6,270 A0488	Good	Marked for Surplus
119273	ESC 8832 A0489	Weigh Lab Room B107	3/1/2004	17	\$6,270 A0489	Good	Marked for Surplus
119274	ESC 8832 A0490	Trailer Dep 3658	3/1/2004	17	\$6,270 A0490	Good	Marked for Surplus
119275	ESC 8832 A0491	Trailer Dep 3658	3/1/2004	17	\$6,270 A0491	Good	Marked for Surplus
119276	ESC 8832 A0492	Trailer Dep 3658	8/12/2004	16	\$6,270 A0492	Good	Marked for Surplus
119277	ESC 8832 A0493	Weigh Lab Room B107	3/1/2004	17	\$6,270 A0493	Good	Marked for Surplus
119278	ESC 8832 A0494	Trailer Dep 3658	3/1/2004	17	\$6,270 A0494	Good	Marked for Surplus
119279	ESC 8832 A0495	Trailer Dep 3658	3/1/2004	17	\$6,270 A0495	Good	Marked for Surplus
119280	ESC 8832 A0496	Trailer Dep 3658	3/1/2004	17	\$6,270 A0496</		

119287	ESC 8832 A0593	MRAS Shop D101	8/12/2004	16	\$6,270 A0593	Good	Active
119288	ESC 8832 A0594	Trailer Dep 3658	5/13/2004	16	\$6,270 A0594	Good	Active
119289	ESC 8832 A0595	Trailer Dep 3658	5/13/2004	16	\$6,270 A0595	Good	Marked for Surplus
119290	ESC 8832 A0596	Trailer Dep 3658	5/13/2004	16	\$6,270 A0596	Good	Marked for Surplus
119291	ESC 8832 A0597	Trailer Dep 3658	5/13/2004	16	\$6,270 A0597	Good	Marked for Surplus
119292	ESC 8832 A0598	Weigh Lab Room B107	5/13/2004	16	\$6,270 A0598	Good	Marked for Surplus
119293	ESC 8832 A0599	Trailer Dep 3658	8/12/2004	16	\$6,270 A0599	Good	Marked for Surplus
119294	ESC 8832 A0600	Trailer Dep 3658	5/13/2004	16	\$6,270 A0600	Good	Active
119295	ESC 8832 A0601	Trailer Dep 3658	5/13/2004	16	\$6,270 A0601	Good	Marked for Surplus
119296	ESC 8832 A0602	Trailer Dep 3658	5/13/2004	16	\$6,270 A0602	Good	Marked for Surplus
119297	ESC 8832 A0603	Broward County	5/13/2004	16	\$7,220 A0603	Good	Active
121305	Envirionics 6103 3285	Trailer Dep 3658	9/1/2004	16	\$12,948.50	3285	Good
121817	R&P 1400AB 140AB253230409	Trailer Dep 3658	11/10/2004	16	\$17,460 140AB253230409	Good	Marked for Surplus
121818	R&P 1400AB 140AB253240409	Trailer Dep 3658	11/10/2004	16	\$17,460 140AB253240409	Good	Marked for Surplus
121819	R&P 1400A 140AB253250409	Trailer Dep 3658	11/10/2004	16	\$17,460 140AB253250409	Good	Marked for Surplus
121882	Dwyer Instruments 475 Mark III MRAS-1	Standards Lab Room B105	10/28/2004	16	\$1,835 MRAS-1	Good	Active
121883	Chinook Engineering FTS MRAS-2	Standards Lab Room B105	10/28/2004	16	\$1,835 MRAS-2	Good	Active
121345	Lightning Master Corporation n/a	A0910002	7/16/2004	16	\$2,810.79 n/a	Good	Active
121346	Lightning Master Corporation n/a	D1056006	7/16/2004	16	\$2,810.80 n/a	Good	Active
Lightning Master Corporation							
121347	101100942	B0890005	7/16/2004	16	\$2,810.80	101100942	Good
121348	Lightning Master Corporation n/a	D1012001	7/16/2004	16	\$2,810.80 n/a	Good	Active
Wells Cargo TW122							
124178	1WC200E2353053636	MRAS Shop Parking Lot	5/16/2005	15	\$9,534.25 1WC200E2353053636	Good	Active
118079	Bios ML 800 101410	Standards Lab Room B105	10/10/2003	17	\$33,075	101410	Good
122462	Opsis 604	Weigh Lab Room B107	5/25/2005	15	\$12,070	604	Good
123902	Opsis n/a	Weigh Lab Room B107	5/25/2005	15	\$4,216 n/a	Good	Active
124758	Fluke 715/87V 8881056	Nature Coast	6/9/2005	15	\$1,081	8881056	Good
124759	Fluke 715/87V 8881048	Forgotten Coast	6/9/2005	15	\$1,081	8881048	Good
124760	Fluke 715/87V 8881046	MRAS Shop D101	6/9/2005	15	\$1,081	8881046	Good
124761	Fluke 715/87V 8881038	MRAS Shop D101A	6/9/2005	15	\$1,081	8881038	Good
124762	Fluke 715/87V 8881043	Lee Island Coast	7/14/2005	15	\$1,081	8881043	Good
124763	Fluke 715/87V 8767140	Sun Coast	7/14/2005	15	\$1,081	8767140	Good
124764	Fluke 715/87V 8767074	Naval Aviation Coast	7/14/2005	15	\$1,081	8767074	Good
124765	Fluke 715/87V 8767090	First Coast	7/14/2005	15	\$1,081	8767090	Good
124766	Fluke 43B DM8860166	MRAS Shop D101	6/9/2005	15	\$1,977.45 DM8860166	Good	Active
117235	Lightning Master Corporation n/a	B0030002	7/17/2003	17	\$2,421.56 n/a	Good	Active
117236	Lightning Master Corporation n/a	D1010005	5/23/2003	17	\$2,421.67 n/a	Good	Active
117237	Lightning Master Corporation n/a	E0210004	7/17/2003	17	\$2,421.56 n/a	Good	Active
125012	R&P 2025 2025B 217930506	Orange County	7/1/2005	15	\$11,890 2025B 217930506	Good	Lost/Missing/Stolen
14796	UltraSonic Bath 220 A1162	MRAS Shop D101	1/1/1980	41	\$500 A1162	Good	Active
20552	Sencore LC 53 3448433M	LabAC-14 Shelf A	1/1/1980	41	\$350 3448433M	Good	Active
122188	NovaLynx 230-355 995472-U1	MRAS Shop D101	8/23/2004	16	\$1,404.69 995472-U1	Good	Active
EPA Supplied	R&P Partisol 2025 2025A202699805	Trailer Dep 3658	7/1/1998	22	\$0 2025A202699805	Good	Marked for Surplus
Lightning Master Corporation							
121000	304005441	MRAS Shop D101	9/27/2004	16	\$2,810	304005441	Good
EPA Supplied	Met One Instruments A2592	G0730012	1/1/2003	18	\$0 A2592	Good	Active
Chinook Engineering Streamline Pro							
133513	M070802	OAM QA Mary Clark	8/28/2007	13	\$3,548 M070802	Good	Active
134321	ESC 8832 A2187	Trailer Dep 3658	1/3/2008	13	\$6,020 A2187	Good	Marked for Surplus
134323	ESC 8832 A2326K	Trailer Dep 3658	1/3/2008	13	\$6,020 A2326K	Good	Marked for Surplus
134322	ESC 8832 A2188	Trailer Dep 3658	1/3/2008	13	\$6,020 A2188	Good	Marked for Surplus
EPA Supplied	R&P Partisol 2025 2025A202709805	L0952002	7/1/1998	22	\$0 2025A202709805	Good	Active
EP006108	Ford Van 1FTNE24W16HA07776	MRAS Shop D101	5/18/2005	15	\$16,887 1FTNE24W16HA07776	Good	Active
126972	AALBORG GFM-17 154938-1	Trailer Dep 3658	2/27/2006	15	\$1,192.25 154938-1	Good	Marked for Surplus
Thermo Environmental Instruments, Inc							
127268	48CTLE 0536 114345	Standards Lab Room B105	3/21/2006	15	\$11,355 0536 114345	Good	In Storage
127465	Mykrolis FC-260V AA06103066	Trailer Dep 3658	3/28/2006	15	\$1,337 AA06103066	Good	Marked for Surplus
127612	ESC 8832 A1289	Broward County	4/21/2006	15	\$6,200 A1289	Good	Active
127613	ESC 8832 A1288	Trailer Dep 3658	4/21/2006	15	\$6,200 A1288	Good	Marked for Surplus
127614	ESC 8832 A1287	Trailer Dep 3658	4/24/2006	15	\$6,200 A1287	Good	Marked for Surplus
127615	ESC 8832 A1286	Trailer Dep 3658	4/21/2006	15	\$6,790 A1286	Good	Marked for Surplus
EPA Supplied	R&P Partisol 2025 2025A203949806	Trailer DNR 2096	7/1/1998	22	\$0 2025A203949806	Good	Marked for Surplus
126973	AALBORG GFM-17 154938-2	Trailer Dep 3658	3/3/2006	15	\$1,154.25 154938-2	Good	Marked for Surplus
127392	Fluke 8505A Multimeter 908852245	Standards Lab Room B105	4/10/2006	15	\$15,532	908852245	Good
127441	Aluma Tower n/a	A0330018	4/3/2006	15	\$2,235 n/a	Good	Active
127442	Aluma Tower T-135-35 n/a	F0850007	5/1/2006	15	\$2,235 n/a	Good	Active
127530	Fluke 715/87V 9015198	Space Coast	5/3/2006	15	\$1,295.05	9015198	Good
127531	Fluke 715/87V 9005307	Space Coast	5/3/2006	15	\$1,295.05	9005307	Good
128028	BK Precision 865 113-01362	Trailer Dep 3658	5/25/2006	14	\$1,090 113-01362	Good	Marked for Surplus
128367	Bios ML 800 108053	Standards Lab Room B105	7/6/2006	14	\$15,155	108053	Good
EPA005552	Ford Expedition 1FMPU15586LA93463	OAM QA Mary Clark	6/30/2006	14	\$23,303.15 1FMPU15586LA93463	Good	Active
ER031036	Aluma Tower n/a	D1056006	11/21/1991	29	\$1,148 n/a	Good	Active
156628	EKTO 432SP 3695-7	Trailer ER015197	5/25/2006	14	\$5,875 3695-7	Good	In Storage
ER030280	EW2011WC22129S	D1012001	10/2/1991	29	\$9,020 EW2011WC22129S	Good	Active
132187	R&P 1400AB 140AB266790704	Trailer Dep 3658	5/15/2007	13	\$24,964 140AB266790704	Good	Marked for Surplus
31033	Aluma Tower na	C0972002	11/21/1991	29	\$1,148 na	Good	Active
Thermo Environmental Instruments, Inc							
132281	49iPS 0714922084	MRAS Shop D101D	5/25/2007	13	\$9,361	714922084	Good
Thermo Environmental Instruments, Inc							
132282	49iPS 0714922083	C1171002	5/25/2007	13	\$7,313	714922083	Good
Thermo Environmental Instruments, Inc		</					

116106	Hastings 16157	OAM QA Room B105	4/21/2003	18	\$1,310	16157	Good	Active
115159	Lightning Master Corporation n/a	A033004	2/25/2003	18	\$8,587.55 n/a		Good	Active
117393	Calibration Bath 803050081	Standards Lab Room B105	6/10/2003	17	\$9,972.90	803050081	Good	Active
Lightning Master Corporation 12100								
115149	202103114	BMC Fenced Lot	12/18/2003	17	\$2,334	202103114	Good	Active
115150	Lightning Master Corporation n/a	C0972002	12/18/2003	17	\$2,334 n/a		Good	Active
Lightning Master Corporation								
115151	202103112	C0690002	1/10/2003	18	\$2,334	202103112	Good	Active
115152	Lightning Master Corporation n/a	LabAC-17 Shelf D	1/10/2003	18	\$2,334 n/a		Good	Active
Lightning Master Corporation								
115153	202103111	B1071008	12/18/2003	17	\$2,334	202103111	Good	Active
Lightning Master Corporation								
115154	202103452	B0013012	12/18/2002	18	\$2,334	202103452	Good	Active
Lightning Master Corporation								
115155	202103451	LabAC-17 Shelf D	12/18/2002	18	\$2,334	202103451	Good	Active
115156	Lightning Master Corporation n/a	E0713002	12/18/2002	18	\$2,334.10 n/a		Good	Active
Lightning Master Corporation		C0090007	1/6/2003	18	\$2,334 n/a		Good	Active
115158	304005441	G0730012	12/18/2002	18	\$2,334	304005441	Good	Active
93876 Bios DC-2 B401	MRAS Shop D101A	12/26/1995	25	\$2,470 B401		Good	Active	
117858 Foil Kit 613	OAM QA Mary Clark	7/17/2003	17	\$1,185	613	Good	Active	
117859 Foil Kit 614	OAM QA Bruce Ferrier	7/17/2003	17	\$1,185	614	Good	Active	
117860 Foil Kit 631	Standards Lab Room B105 Cab D	7/17/2003	17	\$1,185	631	Good	Active	
117238 Environics 16527	OAM QA Room B105	6/5/2003	17	\$1,310	16527	Good	Active	
117239 Environics 16528	OAM QA Room B105	6/5/2003	17	\$1,310	16528	Good	Active	
93874 Bios DC-2NSH B-398	Southwest District Office	12/26/1995	25	\$2,470 B-398		Good	Active	
141349 Dell Optiplex 780 2X955P1	MRAS Shop D101	12/6/2010	10	\$621.90 2X955P1		Good	Active	
141350 Dell Optiplex 780 8YQ74P1	Trailer Dep 3658	12/6/2010	10	\$621.90 8YQ74P1		Good	In Storage	
141352 Dell Optiplex 780 8X955P1	MRAS Shop D101	12/6/2010	10	\$621.90 8X955P1		Good	Active	
141353 Dell Optiplex 780 C9Y74P1	MRAS Shop D101	12/6/2010	10	\$621.90 C9Y74P1		Good	Active	
141354 Dell Optiplex 780 9YQ74P1	LabAC-15 Shelf B	12/6/2010	10	\$621.90 9YQ74P1		Good	Active	
141355 Dell Optiplex 780 CQ955P1	LabAC-15 Shelf A	12/6/2010	10	\$621.90 CQ955P1		Good	In Storage	
141356 Dell Optiplex 780 1Q955P1	LabAC-15 Shelf B	12/6/2010	10	\$621.90 1Q955P1		Good	In Storage	
141357 Dell Optiplex 780 JP955P1	MRAS Shop D101	12/6/2010	10	\$621.90 JP955P1		Good	In Storage	
141358 Dell Optiplex 780 4YQ74P1	MRAS Shop D101	12/6/2010	10	\$621.90 4YQ74P1		Good	In Storage	
141359 Dell Optiplex 780 3BYS3P1	ALabC-14 Shelf C	12/6/2010	10	\$621.90 3BYS3P1		Good	In Storage	
141360 Dell Optiplex 780 G6X74P1	LabAC-15 Shelf A	12/6/2010	10	\$621.90 G6X74P1		Good	In Storage	
141363 Dell Optiplex 780 7Q955P1	Trailer Dep 3658	12/6/2010	10	\$621.90 7Q955P1		Good	Active	
141364 Dell Optiplex 780 29Y74P1	LabAC-15 Shelf A	12/6/2010	10	\$621.90 29Y74P1		Good	In Storage	
141365 Dell Optiplex 780 5BYS3P1	Trailer Dep 3658	12/6/2010	10	\$621.90 5BYS3P1		Good	Active	
141366 Dell Optiplex 780 FQ955P1	LabAC-15 Shelf A	12/6/2010	10	\$621.90 FQ955P1		Good	Marked for Surplus	
141368 Dell Optiplex 780 19Y74P1	MRAS Shop D101	12/6/2010	10	\$621.90 19Y74P1		Good	In Storage	
141369 Dell Optiplex 780 BR955P1	A0330004	12/6/2010	10	\$621.90 BR955P1		Good	Active	
141370 Dell Optiplex 780 H7Y74P1	LabAC-15 Shelf A	12/6/2010	10	\$621.90 H7Y74P1		Good	In Storage	
141371 Dell Optiplex 780 D5X74P1	ALabC-14 Shelf C	12/6/2010	10	\$621.90 D5X74P1		Good	In Storage	
141372 Dell Optiplex 780 2ZQ74P1	MRAS Shop D101	12/6/2010	10	\$621.90 2ZQ74P1		Good	In Storage	
141373 Dell Optiplex 780 BQ955P1	LabA137A	12/6/2010	10	\$621.90 BQ955P1		Good	In Storage	
141375 Dell Optiplex 780 JX974P1	LabAC-15 Shelf A	12/6/2010	10	\$621.90 JX974P1		Good	In Storage	
141377 Dell Optiplex 780 6XQ74P1	MRAS Shop D101	12/6/2010	10	\$621.90 6XQ74P1		Good	In Storage	
141378 Dell Optiplex 780 B5X74P1	LabA137A	12/6/2010	10	\$621.90 B5X74P1		Good	In Storage	
141379 Dell Optiplex 780 CP955P1	MRAS Shop D101	12/6/2010	10	\$621.90 CP955P1		Good	Active	
141380 Dell Optiplex 780 7XQ74P1	MRAS Shop D101	12/6/2010	10	\$621.90 7XQ74P1		Good	Active	
141382 Dell Optiplex 780 GR955P1	MRAS Shop D101B	12/6/2010	10	\$621.90 GR955P1		Good	Active	
141383 Dell Optiplex 780 F9Y74P1	LabAC-15 Shelf A	12/6/2010	10	\$621.90 F9Y74P1		Good	In Storage	
141384 Dell Optiplex 780 H9Y74P1	MRAS Shop D101	12/6/2010	10	\$621.90 H9Y74P1		Good	In Storage	
141386 Dell Optiplex 780 16X74P1	LabAC-15 Shelf A	12/6/2010	10	\$621.90 16X74P1		Good	In Storage	
143515 Vaisala WXT520 G3420011	E0713002	9/2/2011	9	\$2,250 G3420011		Good	Active	
143511 Vaisala WXT520 G3420015	E0210004	9/2/2011	9	\$2,250 G3420015		Good	Active	
143521 Vaisala WXT520 G3420019	ALabC-14 Shelf C	9/2/2011	9	\$2,250 G3420019		Good	In Maintenance	
143522 Vaisala WXT520 G3420023	D1010005	9/2/2011	9	\$2,250 G3420023		Good	Active	
135129 Fluke 715/87V 9612059	MRAS Shop D101	4/8/2008	13	\$1,300.78	9612059	Good	Active	
135128 Fluke 715/87V 9612049	MRAS Shop D101D	4/8/2008	13	\$1,300.78	9612049	Good	Active	
135127 Fluke 715/87V 9612035	Emerald Coast	4/8/2008	13	\$1,300.78	9612035	Good	Active	
135229 eLutions iRX 0809001626	LabAC-15 Shelf C	4/8/2008	13	\$1,116.25	809001626	Good	Marked for Surplus	
135239 Aluma Tower T-135-35 AT-82070-T-4-2	C1171002	4/22/2008	13	\$2,367.50 AT-82070-T-4-2		Good	In Storage	
135231 eLutions iRX 0809001677	LabAC-15 Shelf C	4/8/2008	13	\$1,116.25	809001677	Good	Marked for Surplus	
Wells Cargo EW2011								
135538 1WC200J2383058622	B0350004	5/28/2008	12	\$14,597 1WC200J2383058622		Good	Active	
Wells Cargo EW2011								
135562 1WC200J2583058623	F0850007	5/28/2008	12	\$14,597 1WC200J2583058623		Good	Active	
89697 Aluma Tower T-135-35' n/a	F1110013	10/20/1994	26	\$1,300 n/a		Good	Active	
Thermo Environmental Instruments, Inc								
137051 49I-A1NAA 0820431148	E0210004	7/9/2008	12	\$7,533.50	820431148	Good	In Storage	
Thermo Environmental Instruments, Inc								
137052 49IPS-ANAA 0820430996	A0050006	7/9/2008	12	\$10,165	820430996	Good	Active	
Thermo Environmental Instruments, Inc								
137565 1405 1405A126411212	Standards Lab Room B105	9/5/2008	12	\$17,554 1405A126411212		Good	Active	
EPA Supplied Met One Instruments SASS A2593	LabAC-14	1/1/2003	18	\$0 A2593		Good	In Storage	
Thermo Environmental Instruments, Inc								
Forest Service 1400ab 140AB273530810	Trailer Dep 3658	2/3/2009	12	\$0 140AB273530810		Good	Marked for Surplus	
Chinook Engineering Streamline Pro								
138594 M081204	OAM QA Mary Clark	3/6/2009	12	\$3,917 M081204		Good	Active	
Chinook Engineering Streamline Pro				</				

	Thermo Environmental Instruments, Inc	MRAS Shop D101	5/4/2009	12	\$10,202.76	913235776	Good	Active
139025	49i-PS-ANAA 0913235776	A1130015	5/12/2009	12	\$7,569.45	CM09130039	Good	Active
	Thermo Environmental Instruments, Inc	Trailer Dep 3658	6/29/2009	11	\$15,161.19	2025B225330905	Good	Marked for Surplus
139174	49i-A1NAA CM09130039	Trailer ER015197	6/29/2009	11	\$15,161.19	2025B225320905	Good	Active
	Thermo Environmental Instruments, Inc	MRAS Shop D101	6/29/2009	11	\$17,705.76	1405A204650904	Good	In Storage
139697	2025-AM 2025B225330905	MRAS Shop D101	6/29/2009	11	\$17,705.77	1405A204780905	Good	Active
	Thermo Environmental Instruments, Inc	MRAS Shop D101	6/29/2009	11	\$16,922.25	1WC200J2693059622	Good	Active
139698	2025-AM 2025B225320905	E0713002	6/9/2009	11	\$16,922.25	1WC200J2893059623	Good	Active
	Thermo Environmental Instruments, Inc	D0170006	6/9/2009	11	\$16,922.25	1WC200J2893059623	Good	Active
139699	1405-AVF 1405A204650904	C0972002	5/2/2000	21	\$10,188	1WC200J19Y3043548	Good	Active
	Thermo Environmental Instruments, Inc	G0730012	7/29/2009	11	\$0	3N-B0724	Good	Active
EP021075	Wells Cargo EW2011	Space Coast	7/29/2009	11	\$0	620	Good	Active
1WC00J2693059622	Wells Cargo EW2011	G0730012	7/29/2009	11	\$0	18603	Good	Active
EP021076	Wells Cargo EW2011	MRAS Shop D101	10/15/2009	11	\$16,958.96	703-S	Good	Active
BL605005	1WC200J19Y3043548	MRAS Shop D101	11/20/2009	11	\$12,575.80	2025B225940912	Good	Marked for Surplus
EPA supplied	URG - 3000 3N-B0724	Trailer Dep 3658	11/20/2009	11	\$12,575.80	2025B225910911	Good	Marked for Surplus
EPA Supplied	BGI Incorporated 620	D114A	11/20/2009	11	\$12,575.80	2025B225830910	Good	Marked for Surplus
EPA Supplied	RADNET - HVP - 4004BRL - S 18603	Trailer Dep 3658	11/20/2009	11	\$12,575.81	2025B225930912	Good	Marked for Surplus
140120	Teledyne API 700E 703-S	Trailer Dep 06095	11/20/2009	11	\$12,575.81	2025B225920912	Good	Marked for Surplus
	Thermo Environmental Instruments, Inc	MRAS Shop D101	12/17/2009	11	\$7,936.32	CM09500013	Good	Active
140300	2025B 2025B225940912	MRAS Shop D101	12/17/2009	11	\$7,936.32	CM09500014	Good	Active
	Thermo Environmental Instruments, Inc	Trailer Dep 3658	12/17/2009	11	\$7,936.32	CM09500015	Good	Active
140297	2025B 2025B225910911	MRAS Shop D101	12/17/2009	11	\$7,936.32	CM09500016	Good	Active
	Thermo Environmental Instruments, Inc	D114A	12/17/2009	11	\$7,936.32	CM09500017	Good	Active
140296	2025B 2025B225830910	MRAS Shop D101	12/17/2009	11	\$7,936.32	CM09500018	Good	Active
	Thermo Environmental Instruments, Inc	Trailer Dep 3658	12/17/2009	11	\$7,936.32	CM09500019	Good	Active
140299	2025B 2025B225930912	MRAS Shop D101	12/17/2009	11	\$7,936.32	CM09500020	Good	Active
	Thermo Environmental Instruments, Inc	Trailer Dep 06095	12/17/2009	11	\$7,936.32	CM09500021	Good	Active
140298	2025B 2025B225920912	MRAS Shop D101	12/17/2009	11	\$7,936.32	CM09500022	Good	Active
	Thermo Environmental Instruments, Inc	Trailer Dep 06095	12/17/2009	11	\$7,936.32	CM09500023	Good	Active
140301	49I-A1NAA CM09500013	MRAS Shop D101	12/17/2009	11	\$7,936.32	CM09500014	Good	Active
	Thermo Environmental Instruments, Inc	D1012001	12/17/2009	11	\$7,936.32	CM09500015	Good	Active
140302	49I-A1NAA CM09500014	MRAS Shop D101	12/17/2009	11	\$7,936.32	CM09500016	Good	Active
	Thermo Environmental Instruments, Inc	LabA137A	12/17/2009	11	\$7,936.32	CM09500017	Good	Active
140303	49I-A1NAA CM09500015	MRAS Shop D101	12/17/2009	11	\$7,936.32	CM09500018	Good	Active
	Thermo Environmental Instruments, Inc	MRAS Shop D101	12/17/2009	11	\$7,936.32	CM09500019	Good	Active
140304	49I-A1NAA CM09500016	MRAS Shop D101	12/17/2009	11	\$7,936.32	CM09500020	Good	Active
	Thermo Environmental Instruments, Inc	MRAS Shop D101	12/17/2009	11	\$7,936.33	CM09500021	Good	Active
140305	49I-A1NAA CM09500017	E0713002	12/17/2009	11	\$7,936.33	CM09500022	Good	Active
	Thermo Environmental Instruments, Inc	MRAS Shop D101	12/17/2009	11	\$9,808	935239567	Good	Active
140306	49IPS-ANAA 0935239567	B0030002	2/3/2010	11	\$9,808	935239568	Good	Active
	Thermo Environmental Instruments, Inc	MRAS Shop D101	12/17/2009	11	\$9,808	935239569	Good	Active
140307	49IPS-ANAA 0935239568	A0590004	12/17/2009	11	\$9,808	935239570	Good	Active
	Thermo Environmental Instruments, Inc	A0910002	12/17/2009	11	\$9,808	935239571	Good	Active
140308	49IPS-ANAA 0935239569	B0013012	12/17/2009	11	\$9,808.01	935239571	Good	Active
	Thermo Environmental Instruments, Inc	B1071008	6/16/2010	10	\$15,103	898-S	Good	Active
140617	Teledyne API 700E 898-S	LabA137A	6/16/2010	10	\$15,103	897-S	Good	Active
140619	Teledyne API 700E 897-S	B0890005	6/16/2010	10	\$15,103	895-S	Good	Active
140620	Teledyne API 700E 895-S	Trailer Dep 3658	6/16/2010	10	\$15,103	899-S	Good	Marked for Surplus
140621	Teledyne API 700E 899-S	MRAS Shop D101	6/16/2010	10	\$15,103	900-S	Good	Awaiting Maintenance
140622	Teledyne API 700E 900-S	MRAS Shop D101	6/22/2010	10	\$9,017.50	A3730K	Good	Active
140661	ESC 8832 A3730K	MRAS Shop D101	6/22/2010	10	\$9,017.50	A3731K	Good	Marked for Surplus
140662	ESC 8832 A3731K	Trailer Dep 3658	6/30/2010	10	\$1,767.75	F2620012	Good	Active
140930	Vaisala WXT520 F2620012	B0350004	9/22/2010	10	\$1,890	120467	Good	Marked for Surplus
141098	Bios Definer Model 220 - M 120467	Trailer Dep 3658	9/22/2010	10	\$1,890	120469	Good	Marked for Surplus
141108	Bios Definer Model 220 - M 120469	Trailer Dep 3658	9/22/2010	10	\$1,890	120460	Good	Marked for Surplus
141109	Bios Definer Model 220 - M 120460	Trailer Dep 3658	9/22/2010	10	\$1,890	120461	Good	Active
141110	Bios Definer Model 220 - M 120461	MRAS Shop D101	9/22/2010	10	\$1,890	120827	Good	Marked for Surplus
141111	Bios Definer Model 220 - M 120827	Trailer Dep 3658	9/22/2010	10	\$1,890	120463	Good	Marked for Surplus
141112	Bios Definer Model 220 - M 120463	Trailer Dep 3658	9/22/2010	10	\$1,890	120466	Good	Marked for Surplus
141113	Bios Definer Model 220 - M 120466	Trailer Dep 3658	9/22/2010	10	\$1,890	120470	Good	Marked for Surplus
141114	Bios Definer Model 220 - M 120470	Trailer Dep 3658	9/22/2010	10	\$1,890	120826	Good	Marked for Surplus
141118	Bios Definer Model 220 - M 120826	Trailer Dep 3658	9/22/2010	10	\$1,890	120464	Good	Marked for Surplus
141119	Bios Definer Model 220 - M 120464	Trailer Dep 3658	11/17/2010	10	\$1,890	120462	Good	Active
141120	Bios Definer Model 220 - M 120462	Central District Office	11/17/2010	10	\$1,890	120468	Good	Marked for Surplus
141121	Bios Definer Model 220 - M 120468	Trailer Dep 3658	11/17/2010	10	\$1,890	120465	Good	Marked for Surplus
141122	Bios Definer Model 220 - M 120465	Trailer Dep 3658	11/17/2010	10	\$1,890	120535	Good	Marked for Surplus
141124	Bios Definer Model 220 - H 120535	Trailer Dep 3658	11/17/2010	10	\$1,890	120540	Good	Marked for Surplus
141125	Bios Definer Model 220 - H 120540	Trailer Dep 3658	11/17/2010	10	\$1,890	120544	Good	Marked for Surplus
141126	Bios Definer Model 220 - H 120544	Trailer Dep 3658	11/17/2010	10	\$1,890	120537	Good	Active
141130	Bios Definer Model 220 - H 120537	MRAS Shop D101	11/17/2010	10	\$1,890	120787	Good	Marked for Surplus
141131	Bios Definer Model 220 - H 120787	Trailer Dep 3658	11/17/2010	10	\$1,890.99	120788	Good	Marked for Surplus
141132	B							

142181	Vaisala WXT520 G0350004	C0830003	1/31/2011	10	\$2,370	G0350004	Good	Active	
142182	Vaisala WXT520 G0350005	A1130015	1/31/2011	10	\$2,370	G0350005	Good	Active	
142183	Vaisala WXT520 G0350006	MRAS Shop D101	1/31/2011	10	\$2,370	G0350006	Good	Active	
142184	Vaisala WXT520 G0350007	A0330018	1/31/2011	10	\$2,370	G0350007	Good	Active	
142185	Vaisala WXT520 G0350008	B0470015	1/31/2011	10	\$2,370	G0350008	Good	Active	
142186	Vaisala WXT520 G0350009	Trailer Dep 3658	1/31/2011	10	\$2,370	G0350009	Good	Marked for Surplus	
142187	Vaisala WXT520 G0350010	B1071008	1/31/2011	10	\$2,370	G0350010	Good	Active	
142188	Vaisala WXT520 G0350011	MRAS Shop D101	1/31/2011	10	\$2,370	G0350011	Good	Active	
142189	Vaisala WXT520 G0350012	MRAS Shop D101	1/31/2011	10	\$2,370	G0350012	Good	Active	
142190	Vaisala WXT520 G0350013	MRAS Shop D101	1/31/2011	10	\$2,370	G0350013	Good	Active	
142191	Vaisala WXT520 G0350014	A0910002	1/31/2011	10	\$2,370	G0350014	Good	Active	
142192	Vaisala WXT520 G0350015	MRAS Shop D101	1/31/2011	10	\$2,370	G0350015	Good	Active	
Not Required	Vaisala WSP150 F5030016	D1056006	1/31/2011	10	\$268	F5030016	Good	Active	
Not Required	Vaisala WSP150 F5030013	MRAS Shop D101	1/31/2011	10	\$268	F5030013	Good	Active	
Not Required	Vaisala WSP150 F5030001	C0830003	1/31/2011	10	\$268	F5030001	Good	Active	
Not Required	Vaisala WSP150 F5030012	MRAS Shop D101	1/31/2011	10	\$268	F5030012	Good	Active	
Not Required	Vaisala WSP150 F5030022	Weigh Lab Room B107	1/31/2011	10	\$268	F5030022	Good	Active	
Not Required	Vaisala WSP150 F5030014	B0470015	1/31/2011	10	\$268	F5030014	Good	Active	
Not Required	Vaisala WSP150 F5030003	B0350004	1/31/2011	10	\$268	F5030003	Good	Active	
Not Required	Vaisala WSP150 F5030008	G0730012	1/31/2011	10	\$268	F5030008	Good	Active	
Not Required	Vaisala WSP150 F5030025	A0330004	1/31/2011	10	\$268	F5030025	Good	Active	
Not Required	Vaisala WSP150 F5030019	Weigh Lab Room B107	1/31/2011	10	\$268	F5030019	Good	Active	
Not Required	Vaisala WSP150 F5030024	A0330018	1/31/2011	10	\$268	F5030024	Good	Active	
Not Required	Vaisala WSP150 F5030021	B0030002	1/31/2011	10	\$268	F5030021	Good	Active	
Not Required	Vaisala WSP150 F5030011	MRAS Shop D101	1/31/2011	10	\$268	F5030011	Good	Active	
Not Required	Vaisala WSP150 F5030023	MRAS Shop D101	1/31/2011	10	\$268	F5030023	Good	Active	
Not Required	Vaisala WSP150 F5030006	Weigh Lab Room B107	1/31/2011	10	\$268	F5030006	Good	In Storage	
Not Required	Vaisala WSP150 F5030017	MRAS Shop D101	1/31/2011	10	\$268	F5030017	Good	In Maintenance	
142160	Teledyne API T400 0083	L0860019	1/21/2011	10	\$7,819.25		83	Good	Active
142161	Teledyne API T400 0084	L1030004	1/21/2011	10	\$7,819.25		84	Good	Active
142162	Teledyne API T400 0085	L1030004	1/21/2011	10	\$7,819.25		85	Good	Active
142163	Teledyne API T400 0086	L0860019	1/21/2011	10	\$7,819.25		86	Good	Active
142164	Teledyne API T400 0087	D114A	1/21/2011	10	\$7,819.25		87	Good	In Storage
Thermo Environmental Instruments, Inc									
142256	2025B 2025B227811103	D114A	3/23/2011	10	\$13,611.45	2025B227811103	Good	Marked for Surplus	
142165	Teledyne API M701 Opt 86E 3412	Trailer Dep 3658	1/10/2011	10	\$4,057.13		3412	Good	Active
142166	Teledyne API M701 Opt 86E 3413	MRAS Shop D101	1/10/2011	10	\$4,057.13		3413	Good	Active
142167	Teledyne API M701 Opt 86E 3414	D0170006	1/10/2011	10	\$4,057.13		3414	Good	Active
142168	Teledyne API M701 Opt 86E 3415	D0810028	1/10/2011	10	\$4,057.13		3415	Good	Active
142169	Teledyne API M701 Opt 86E 3416	MRAS Shop D101	1/10/2011	10	\$4,057.13		3416	Good	Active
142170	Teledyne API M701 Opt 86E 3418	Trailer Dep 3658	1/10/2011	10	\$4,057.13		3418	Good	Marked for Surplus
142171	Teledyne API M701 Opt 86E 3419	Surplus Trailer	1/10/2011	10	\$4,057.13		3419	Good	Marked for Surplus
142172	Teledyne API M701 Opt 86E 3420	D1056005	1/10/2011	10	\$4,057.13		3420	Good	Active
142173	Teledyne API M701 Opt 86E 3421	Trailer Dep 3658	1/10/2011	10	\$4,057.13		3421	Good	Marked for Surplus
142174	Teledyne API M701 Opt 86E 3422	B0890005	1/10/2011	10	\$4,057.13		3422	Good	Active
142176	Teledyne API M701 Opt 86E 3424	MRAS Shop D101A	1/11/2011	10	\$4,057.13		3424	Good	In Storage
142203	Teledyne API T703 057	D114A	2/4/2011	10	\$9,757.51		57	Good	Cannibalized
142204	Teledyne API T703 058	L1030004	2/4/2011	10	\$9,757.51		58	Good	Active
142205	Teledyne API T703 059	D114A	2/4/2011	10	\$9,757.51		59	Good	Cannibalized
142206	Teledyne API T703 060	L0860019	2/4/2011	10	\$9,757.51		60	Good	Active
142207	Teledyne API T703 061	L1030004	2/4/2011	10	\$9,757.51		61	Good	Active
142312	Teledyne API T100 0114	L0118002	5/2/2011	10	\$10,211.35		114	Good	Active
141344	Dell Optiplex 780 H8Y74P1	LabAC-15 Shelf A	12/6/2010	10	\$621.90	H8Y74P1	Good	In Storage	
141345	Dell Optiplex 780 HW955P1	ALabC-14 Shelf C	12/6/2010	10	\$621.90	HW955P1	Good	Active	
141346	Dell Optiplex 780 GP955P1	LabA137A	12/6/2010	10	\$621.90	GP955P1	Good	In Storage	
141351	Dell Optiplex 780 J8Y74P1	MRAS Shop D101	12/6/2010	10	\$621.90	J8Y74P1	Good	Active	
141367	Dell Optiplex 780 J7Y74P1	MRAS Shop D101	12/6/2010	10	\$621.90	J7Y74P1	Good	Active	
141376	Dell Optiplex 780 D9Y74P1	LabAC-15 Shelf A	12/6/2010	10	\$621.90	D9Y74P1	Good	In Storage	
141381	Dell Optiplex 780 1ZQ74P1	LabAC-15 Shelf A	12/6/2010	10	\$621.90	1ZQ74P1	Good	In Storage	
141385	Dell Optiplex 780 88Y74P1	LabAC-15 Shelf A	12/6/2010	10	\$621.90	88Y74P1	Good	In Storage	
141347	Dell Optiplex 780 1S955P1	LabAC-15 Shelf A	12/6/2010	10	\$621.90	1S955P1	Good	In Storage	
141348	Dell Optiplex 780 FP955P1	MRAS Shop D101	12/6/2010	10	\$621.90	FP955P1	Good	In Storage	
141361	Dell Optiplex 780	MRAS Shop D101	12/6/2010	10	\$621.90		Good	In Storage	
141374	Dell Optiplex 780	MRAS Shop D101	12/6/2010	10	\$621.90		Good	In Storage	
54321	Dell		9/27/2012	8	\$0		Good	In Storage	
Thermo Environmental Instruments, Inc									
145216	49i 1227254949	MRAS Shop D101	9/5/2012	8	\$8,441.78		1227254949	Good	Awaiting Maintenance
Thermo Environmental Instruments, Inc									
145217	49i 1227254943	C0972002	9/5/2012	8	\$8,441.78		1227254943	Good	Active
Thermo Environmental Instruments, Inc									
145218	49i 1227254945	C0690002	9/5/2012	8	\$8,441.78		1227254945	Good	Active
Thermo Environmental Instruments, Inc									
145219	49i 1227254948	A0330004	9/5/2012	8	\$8,441.78		1227254948	Good	Active
Thermo Environmental Instruments, Inc									
145220	49i 1227254942	C0830003	9/5/2012	8	\$8,441.78		1227254942	Good	Active
Thermo Environmental Instruments, Inc									

	155460 Agilaire LLC 8872 0865	C0972002	2/21/2019	2	\$8,550	865	Good	Active
	155461 Agilaire LLC 8872 0866	F0850007	2/21/2019	2	\$8,550	866	Good	Active
	155462 Agilaire LLC 8872 0867	F1110013	2/21/2019	2	\$0	867	Good	Active
	155463 Agilaire LLC 8872 0868	MRAS Shop D101	2/21/2019	2	\$8,550	868	Good	Active
	155464 Agilaire LLC 8872 0869	MRAS Shop D101	2/21/2019	2	\$8,550	869	Good	In Maintenance
	155465 Agilaire LLC 8872 0870	C0690002	2/21/2019	2	\$8,550	870	Good	Active
	155466 Agilaire LLC 8872 0871	B0470015	2/21/2019	2	\$8,550	871	Good	Active
	155467 Agilaire LLC 8872 0872	D1056006	2/21/2019	2	\$8,550	872	Good	Active
	155468 Agilaire LLC 8872 0873	MRAS Shop D101	2/21/2019	2	\$8,550	873	Good	In Maintenance
	155469 Agilaire LLC 8872 0874	MRAS Shop D101	2/21/2019	2	\$8,550	874	Good	Active
	Thermo Fisher Scientific 146IQ							
	155517 1182980003	MRAS Shop D101	2/28/2019	2	\$21,107.73	1182980003	Good	In Maintenance
	156236 NovaLynx M202-AI0038 1921000073	Standards Lab Room B105	4/18/2019	2	\$1,630	1921000073	Good	In Storage
	156235 NovaLynx M202-AI0038 1918000075	Standards Lab Room B105	4/18/2019	2	\$1,630	1918000075	Good	Active
	156234 NovaLynx M202-AI0038 1918000074	Standards Lab Room B105	4/18/2019	2	\$1,630	1918000074	Good	Active
	136476 NovaLynx 230-355 914761-J4	Sun Coast	5/15/2015	5	\$1,404.69	914761-J4	Good	Active
	136477 NovaLynx 355-A10900 914762-J3	Emerald Coast	5/15/2015	5	\$1,404.69	914762-J3	Good	Active
	136478 NovaLynx 355-A10900 914762-J4	Nature Coast	5/15/2015	5	\$1,404.69	914762-J4	Good	Active
	149468 Teledyne API T700U 242	Standards Lab Room B105	5/20/2015	5	\$21,510.90	242	Good	Active
	149485 Agilaire LLC 8872 0458	MRAS Shop D101	6/16/2015	5	\$6,950	458	Good	Active
	149486 Agilaire LLC 8872 0459	G1290001	6/16/2015	5	\$6,950	459	Good	Active
	149487 Agilaire LLC 8872 0460	MRAS Shop D101	6/16/2015	5	\$6,950	460	Good	Active
	149488 Agilaire LLC 8872 0461	B0030002	6/16/2015	5	\$6,950	461	Good	Active
	149489 Agilaire LLC 8872 0462	MRAS Shop D101	6/16/2015	5	\$6,950	462	Good	Active
	149558 Teledyne API T750U 56	Standards Lab Room B105	7/15/2015	5	\$21,387.90	56	Good	Active
	149560 Teledyne API T750U 58	OAM QA Mary Clark	7/15/2015	5	\$23,387.90	58	Good	Active
	149631 Agilaire LLC 8872 0489	MRAS Shop D101	9/14/2015	5	\$6,950	489	Good	In Maintenance
	149632 Agilaire LLC 8872 0487	MRAS Shop D101	9/15/2015	5	\$6,950	487	Good	Active
	149630 Agilaire LLC 8872 0488	B0890005	9/15/2015	5	\$6,950	488	Good	Active
	149633 Agilaire LLC 8872 0490	C1171002	9/15/2015	5	\$6,950	490	Good	Active
	Thermo Environmental Instruments, Inc							
	149827 43I So2 Analyzer JC 1526101643	LabA137A	11/9/2015	5	\$11,497.28	JC 1526101643	Good	In Storage
	Thermo Environmental Instruments, Inc							
	149826 43I So2 Analyzer JC 1526101647	B0470015	11/9/2015	5	\$11,497.28	JC 1526101647	Good	Active
	149904 Teledyne API M602B SN 182	D114A	11/16/2015	5	\$0	SN 182	Good	In Storage
	149905 Teledyne API M602B SN 183	D114A	11/16/2015	5	\$0	SN 183	Good	In Storage
	149906 Teledyne API M602B SN 184	D114A	11/16/2015	5	\$0	SN 184	Good	In Storage
	Thermo Environmental Instruments, Inc							
	149977 1405 1405A232741511	B0470015	10/12/2015	5	\$16,881.22	1405A232741511	Good	Active
	Thermo Environmental Instruments, Inc							
	149978 1405 1405A232711510	B0230002	10/12/2015	5	\$16,881.22	1405A232711510	Good	Active
	Thermo Environmental Instruments, Inc							
	149979 1405 1405A232961511	MRAS Shop D101	10/12/2015	5	\$16,881.22	1405A232961511	Good	Active
	Thermo Environmental Instruments, Inc							
	149980 1405 1405A232801511	A1130015	10/12/2015	5	\$16,881.22	1405A232801511	Good	Active
	Thermo Environmental Instruments, Inc							
	149981 1405 1405A232951511	D0170006	10/12/2015	5	\$16,881.22	1405A232951511	Good	Active
	150107 Teledyne API T700 2328	D1056005	1/19/2016	5	\$0	2328	Good	Active
	150106 Teledyne API T700 2329	D0170006	1/19/2016	5	\$0	2329	Good	Active
	150105 Teledyne API T700 2330	A0330004	1/19/2016	5	\$0	2330	Good	Active
	Novalynx 355-AI0900-04103003							
	117940 976370-T2	Naval Aviation Coast	6/23/2016	4	\$0	976370-T2	Good	Active
N/A	Fluke 87 V 96390268	Lee Island Coast	8/4/2016	4	\$0	96390268	Good	Active
N/A	Fluke 77 II 5290515		9/23/2016	4	\$0	5290515	Good	Active
	151133 BGI Incorporated tetracal 151503	MRAS Shop D101	10/6/2016	4	\$2,549.80	151503	Good	Active
	151135 BGI Incorporated tetracal 151498	Space Coast	10/6/2016	4	\$2,549.80	151498	Good	Active
	151131 BGI Incorporated tetracal 151505	Lee Island Coast	10/6/2016	4	\$2,549.80	151505	Good	Active
	151137 BGI Incorporated tetracal 151504	Sun Coast	10/6/2016	4	\$2,549.80	151504	Good	Active
	151134 BGI Incorporated tetracal 151509	First Coast	10/6/2016	4	\$2,549.80	151509	Good	Active
	151138 BGI Incorporated tetracal 151493	Nature Coast	10/6/2016	4	\$2,549.80	151493	Good	Active
	151132 BGI Incorporated tetracal 151494	Naval Aviation Coast	10/6/2016	4	\$2,549.80	151494	Good	Active
	151136 BGI Incorporated tetracal 151500	Emerald Coast	10/6/2016	4	\$2,549.80	151500	Good	Active
	149559 Teledyne API T750U 57	Standards Lab Room B105	6/1/2015	5	\$23,137.50	57	Good	Active
N/A	Dwyer Instruments 475 01NW1	Standards Lab Room B105	10/27/2016	4	\$0	01NW1	Good	Active
N/A	Fluke 87 V 88700898		10/28/2016	4	\$0	88700898	Good	Active
N/A	DM384 U843100063		3/9/2017	4	\$0	U843100063	Good	Active
	140038 Fluke 8845A 1058017	Standards Lab Room B105	5/1/2017	4	\$0	1058017	Good	Active
	140037 Fluke 8845A 1058016	Standards Lab Room B105	5/1/2017	4	\$0	1058016	Good	Active
	152008 Teledyne API T750U 99	OAM QA Bruce Ferrier	5/12/2017	4	\$0	99	Good	Active
	Thermo Fisher Scientific 2025i-AN							
	152054 2025iW2 1192 1704	D114A	5/30/2017	3	\$0	2025iW2 1192 1704	Good	In Storage
	152395 Teledyne API T 640 182	LabA137A	6/5/2017	3	\$23,799.20	182	Good	Active
	152396 Teledyne API T 640 183	MRAS Shop D101	6/5/2017	3	\$23,799.20	183	Good	In Maintenance
	152397 Teledyne API T 640 184	LabA137A	6/5/2017	3	\$23,799.20	184	Good	Active
	152398 Teledyne API T 640 185	MRAS Shop D101	6/5/2017	3	\$23,799.20	185	Good	In Maintenance
	152399 Teledyne API T 640 186	E0710005	6/5/2017	3	\$23,799.20	186	Good	Active
	Thermo Fisher Scientific 1405							
	152012 1405A239061703	D1056006	6/7/2017	3	\$20,264.42	1405A239061703	Good	Active
	152635 Teledyne API T100u 278	G1290001	7/18/2017	3	\$0	278	Good	Active
	152472 Teledyne API T 300U 378	MRAS Shop D101	7/18/2017	3	\$0	378	Good	Active
	152604 Agilaire LLC 8872 0717	MRAS Shop D101	7/17/2017	3	\$6,795	717	Good	Active
	152605 Agilaire LLC 8872 0718	G0730012	7/17/2017	3	\$6,795	7		

157943 Agilaire LLC 8872 1033	B0350004	4/20/2020	1	\$7,737	1033	Good	Active
157944 Agilaire LLC 8872 1034	B0230002	4/20/2020	1	\$7,737	1034	Good	Active
157945 Agilaire LLC 8872 1035	D1010005	4/20/2020	1	\$7,737	1035	Good	Active
157946 Agilaire LLC 8872 1036 Thermo Fisher Scientific 146IQ	C0090007	4/20/2020	1	\$7,737	1036	Good	Active
156751 1191843415 Thermo Fisher Scientific 146IQ	MRAS Shop D101	8/31/2020	0	\$0	1191843415	Good	In Maintenance
156719 1181030049 Thermo Fisher Scientific 49IQ	MRAS Shop D101	8/31/2020	0	\$0	1181030049	Good	In Maintenance
157450 1200937048 Thermo Fisher Scientific 1405	G0730012	5/1/2020	1	\$10,802.98	1200937048	Good	Active
156667 1405A243961907		5/1/2019	2	\$18,000	1405A243961907	Good	Active
157985 Teledyne API T640 1045	B0013012	10/5/2020	0	\$22,595	1045	Good	Active
156237 NovaLynx M202-AI0038 1921000074	OAM QA Mary Clark	4/18/2019	2	\$1,630	1921000074	Good	Active
156180 NovaLynx M202-AI0038 1918000073	OAM QA Bruce Ferrier	4/18/2019	2	\$1,630	1918000073	Good	Active
156189 Mesa Labs ML-800 172051	Standards Lab Room B105	5/21/2019	1	\$6,800	172051	Good	Active
156190 Mesa Labs ML-800 High Cell 170560 Mesa Labs ML-800 Medium Cell	Standards Lab Room B105	5/21/2019	1	\$11,000	170560	Good	Active
156191 171983	Standards Lab Room B105	5/21/2019	1	\$11,000	171983	Good	Active
156192 Mesa Labs ML-800 Low Cell 170275	Standards Lab Room B105	5/21/2019	1	\$11,000	170275	Good	Active
156193 Mesa Labs ML-800 Ultra Low 170812	Standards Lab Room B105	5/21/2019	1	\$18,500	170812	Good	Active
154569 Teledyne API 751H 241	Standards Lab Room B105	6/27/2019	1	\$0	241	Good	Active
156542 Teledyne API 751H 303	OAM QA Bruce Ferrier	6/27/2019	1	\$0	303	Good	Active
154567 Teledyne API 751H 239	Standards Lab Room B105	6/27/2019	1	\$0	239	Good	Active
154568 Teledyne API 751H 240	Standards Lab Room B105	6/27/2019	1	\$0	240	Good	Active
154570 Teledyne API 751H 242	OAM QA Mary Clark	6/27/2019	1	\$0	242	Good	Active
156540 Teledyne API T 640X 713	A0330004	6/28/2019	1	\$0	713	Good	In Storage
156596 Agilaire LLC 8872 0914	E0550003	7/8/2019	1	\$7,695	914	Good	Active
156597 Agilaire LLC 8872 0915	D1012001	7/8/2019	1	\$7,695	915	Good	Active
156598 Agilaire LLC 8872 0916	E0713002	7/8/2019	1	\$7,695	916	Good	Active
156599 Agilaire LLC 8872 0917	D0810028	7/8/2019	1	\$7,695	917	Good	Active
156600 Agilaire LLC 8872 0918	E0712002	7/8/2019	1	\$7,695	918	Good	Active
156601 Agilaire LLC 8872 0919	E0210004	7/8/2019	1	\$7,695	919	Good	Active
156602 Agilaire LLC 8872 0920	D1056005	7/8/2019	1	\$7,695	920	Good	Active
156603 Agilaire LLC 8872 0921	C0094001	7/8/2019	1	\$7,695	921	Good	Active

Manatee County										
Property /Identification No.	Manufacturer and Model No.	Description	Location	Serial No.	Acquisition Date	Age	Initial Cost	Condition	Status	
N/A	Thermo 49i PS	PS	Port	1311657726	2011	10	\$10,417.00	Good	Active	
N/A	Thermo 49i PS	PS	39th	1116648522	2011	10	\$10,417.00	Good	Active	
N/A	Thermo 49i PS	PS	Gt Bray	1023843898	2013	8	\$10,417.00	Good	Active	
N/A	2b Technologies 211	O3 monitor	Gt Bray	34	2020	1	\$14,000.00	Good	Active	
N/A	2b Technologies 202	O3 monitor	Office	903	2010	11	\$5,000.00	Good	Backup	
N/A	2b Technologies 202	O3 monitor	Office	1221	2012	9	\$5,000.00	Good	Active	
N/A	2b Technologies 202	O3 monitor	39th	1092	2011	10	\$5,000.00	Good	Active	
N/A	2b Technologies 202	O3 monitor	office	1094	2011	10	\$5,000.00	Good	Backup	
N/A	ESC Datalogger 8872 (w10)	Data logger	office	1013	2020	1	\$8,285.00	Good	active	
N/A	ESC Datalogger 8872	Data logger	39th	8872_385	2014	7	\$7,640.00	Good	backup	
N/A	ESC Datalogger 8872	Data logger	Gt Bray	8872_0796	2017	4	\$7,640.00	Good	Active	
N/A	ESC Datalogger 8872 (w10)	Data logger	Port	8872_0854	2018	3	\$7,640.00	Good	Active	
N/A	ESC Datalogger 8832	Data logger	Office	A4002K	2012	9	\$7,640.00	Good	Backup	
N/A	ESC Datalogger 8832	Data logger	office	A1583K	2006	15	\$7,640.00	Good	Backup	
N/A	ESC Datalogger 8832	Data logger	office	A3763k	2011	10	\$7,640.00	Good	Backup	
N/A	RM Young 85000	Anenometer	Port	N/A	2011	10	\$1,390.00	Good	Active	
N/A	RM Young 85000	Anenometer	Gt Bray	N/A	2011	10	\$1,390.00	Good	Active	
N/A	RM Young 85000	Anenometer	39th	N/A	2013	8	\$1,390.00	Good	Active	
N/A	Fluke 51 II	Thermometer	office	14390153	2010	11	\$270.00	Good	Active	
N/A	Bios 220 Definer	flow sensor	office	135621	2014	7	\$2,125.00	Good	Active	
N/A	Fluke 715	voltage generator	office	2799124	2014	7	\$1,200.00	Good	Active	
N/A	Fluke 175	volt meter	office	41440651	2018	3	\$300.00	Good	Active	
N/A	Fluke 175	volt meter	office	15880829	2011	10	\$300.00	Good	Active	
N/A	Fluke 1623-2	Ground tester	office	St144506177B2	2012	9	\$2,700.00	Good	Active	
N/A	Air Monitoring shelter	Shelter	Gt Bray	N/A	2016	5	\$24,651.00	Good	Active	
N/A	Air Monitoring shelter	Shelter	Port	N/A	2012	9	\$16,275.00	Good	Active	
N/A	Air Monitoring Trailer	Shelter	39th	N/A	1998	23	\$18,335.00	Fair	Active	
N/A	Gast 1HAB-11T-M100x	Zero Air	Gt Bray	N/A	2018	3	\$1,082.05	Good	Active	
N/A	Gast 1HAB-11T-M100x	Zero Air	Port	N/A	2018	3	\$1,082.05	Good	Active	
N/A	Gast 1HAB-11T-M100x	Zero Air	39th	N/A	2018	3	\$1,082.05	Good	Active	
N/A	Gast 1HAB-11T-M100x	Zero Air	Gt Bray	N/A	Unknown	unknown	\$1,082.05	Fair	Backup	
N/A	Gast 1HAB-11T-M100x	Zero Air	Port	N/A	Unknown	unknown	\$1,082.05	Fair	Backup	
N/A	Gast 1HAB-11T-M100x	Zero Air	39th	N/A	Unknown	unknown	\$1,082.05	Fair	Backup	
N/A	Gast 1HAB-11T-M100x	Zero Air	office	N/A	Unknown	unknown	\$1,082.05	Fair	Backup	
N/A	Omega 303AV	Shelter Tem	Port	60637	2018	3	\$330.00	Good	Active	
N/A	Omega 303AV	Shelter Tem	39th	60640	2018	3	\$330.00	Good	Active	
N/A	Omega 303AV	Shelter Tem	Gt Bray	60937	2018	3	\$330.00	Good	Active	
N/A	LabComp ATX	Shelter temp	Gt Bray	182	Unknown	unknown	\$255.00	Fair	Backup	
N/A	LabComp ATX	Shelter temp	Port	183	Unknown	unknown	\$255.00	Fair	Backup	
N/A	LabComp ATX	Shelter temp	39th	189	Unknown	unknown	\$255.00	Fair	Backup	
N/A	Extech AN400	Anenometer	Office	N/A	Unknown	unknown	\$189.00	Fair	Active	
N/A	Glen Martin MF1331	Met Tower	Port	N/A	2016	5	\$5,260.00	Good	Active	
N/A	Glen Martin MF1331	Met Tower	Gt Bray	N/A	1998	23	\$5,260.00	Fair	Active	
N/A	Glen Martin MF1331	Met Tower	39th	N/A	1998	23	\$5,260.00	Fair	Active	
N/A	Omega HX93bv1-D	Temp Sensor	office	N/A	2015	6	\$255.00	Good	Backup	
N/A	Omega HX93bv1-D	Temp Sensor	office	N/A	2013	8	\$255.00	Good	Backup	
N/A	AlrLink MG90	Communications	Gt Bray	295717601	2020	1	\$1,669.00	Good	Active	
N/A	AlrLink GX400	Communications	39th	295705401	2020	1	\$1,169.00	Good	Active	
N/A	AlrLink GX400	Communications	Port	202733901	2020	1	\$1,669.00	Good	Active	
N/A	AlrLink GX400	Communications	Gt Bray	N/A	2012	9	\$1,669.00	Good	Active	
N/A	AlrLink GX400	Communications	Port	N/A	2012	9	\$750.00	Good	Active	
N/A	AlrLink GX400	Communications	39th	N/A	2012	9	\$750.00	Good	Active	
N/A	Various	Dehumidifier	39th	N/A	Unknown	unknown	\$230.00	fair	Active	
N/A	Various	Dehumidifier	Port	N/A	Unknown	unknown	\$230.00	fair	Active	
N/A	Various	Dehumidifier	Gt Bray	N/A	Unknown	unknown	\$230.00	fair	Active	
N/A	RM Young	Rain gauge	39th	N/A	2019	2	\$600.00	fair	Active	
N/A	RM Young	Rain gauge	Port	N/A	2019	2	\$600.00	fair	Active	
N/A	RM Young	Rain gauge	Gt Bray	N/A	2019	2	\$600.00	fair	Active	
N/A	Oakton 03316-72	barometer	Office	880891	2019	2	\$230.00	Broken	Active	

Pinellas County 2020_2021

Property /Identification No.	Manufacturer and Model No.	Description	Location	Serial No.	Acquisition Date	Age	Initial Cost	Condition	Status
n/a	T-API T400	Ozone	12-103-0004	6021	9/30/2020	0.3	8,600	Good	Deployed
n/a	T-API T640	PM 2.5	12-103-0004	890	2/10/2020	1.2	23,820	Good	Deployed
n/a	T-API T703	O ₃ Primary	12-103-0004	729	8/1/2019	1.8	11,700	Good	Deployed
n/a	Agilaire 8872	data logger	12-103-0004	0412	4/2/2015	6.5	6,600	Good	Deployed
n/a	G&S	Building	12-103-0004	n/a	3/7/1986	35.2	3,500	Good	Deployed
n/a	Met One E-BAM Plus	PM 10	12-103-0012	X19178	9/17/2018	2.6	8,310	Good	Deployed
n/a	T-API T700U	Calibrator	12-103-0018	649	9/30/2020	0.3	23,760	Good	Deployed
n/a	T-API T500U	NO ₂	12-103-0018	304	9/30/2020	0.3	17,200	Good	Deployed
n/a	T-API T640X	PM 2.5/ 10	12-103-0018	218	8/24/2017	3.7	28,200	Good	Deployed
n/a	T-API T400	Ozone	12-103-0018	3071	5/17/2017	3.8	8,102	Good	Deployed
n/a	T-API 701H	Zero Air	12-103-0018	240	8/19/2016	4.7	8,000	Good	Deployed
n/a	Agilaire 8872	data logger	12-103-0018	0310	8/27/2014	6.5	6,600	Good	Deployed
n/a	RM Young 5305	Wind sensor	12-103-0018	54915	n/a	9	1,100	Good	Deployed
n/a	Robin Builders	Building	12-103-0018	n/a	1/28/1998	23.3	14,142	Fair	Deployed
n/a	Aluma Tower 10m	wind tower	12-103-0018	na	8/28/1989	31.7	2,000	Fair	Deployed
n/a	T-API T703	O ₃ Primary	12-103-0018	61	n/a	n/a	n/a	Good	Deployed
n/a	Envirronics 7000	Zero Air	12-103-0023	8640	9/10/2019	1.6	4,700	Good	Deployed
n/a	TEI 43i	SO ₂	12-103-0023	1163630020	12/14/2016	4.2	12,500	Good	Deployed
n/a	Envirronics 6100	Calibrator	12-103-0023	6551	6/1/2015	5.9	8,900	Good	Deployed
n/a	Agilaire 8872	data logger	12-103-0023	0309	8/27/2014	6.5	6,600	Good	Deployed
n/a	William Scottsman	Building	12-103-0023	n/a	9/26/1997	23.6	11,400	Fair	Deployed
n/a	RM Young 5305	Wind sensor	12-103-0026	57347	n/a	6	1,100	Good	Deployed
n/a	Agilaire 8872	data logger	12-103-0026	0411	8/27/2014	6.5	6,600	Good	Deployed
n/a	T-API/Magee 633	Aethalometer	12-103-0026	AE33-S01-00107	6/11/2013	7.9	11,000	Good	Deployed
n/a	Aluma Tower 10m	wind tower	12-103-0026	na	8/21/2001	19.7	2,000	Fair	Deployed
n/a	Robin Builders	Building	12-103-0026	n/a	12/12/1997	23.4	10,800	Fair	Deployed
n/a	T-API T700U	Calibrator	12-103-0027	251	5/20/2016	5.0	21,400	Good	Deployed
n/a	T-API 701H	Zero Air	12-103-0027	136	5/20/2016	5.0	8,000	Good	Deployed
n/a	T-API/Magee 633	Aethalometer	12-103-0027	AE33-S03-00336	5/20/2016	5.0	7,200	Good	Deployed
n/a	T-API T500U	NO ₂	12-103-0027	108	5/20/2016	4.8	16,000	Good	Deployed
n/a	T-API T300U	CO	12-103-0027	242	5/20/2016	4.8	12,700	Good	Deployed
n/a	William Scottsman	Building	12-103-0027	n/a	1/1/2016	5.3	27,500	Good	Deployed
n/a	Aluma Tower 10m	wind tower	12-103-0027	na	9/30/2015	5.6	4,100	Good	Deployed
n/a	Envirronics 6100	Calibrator	12-103-0027	6552	6/1/2015	5.9	8,900	Good	Deployed
n/a	RM Young 5305	Wind sensor	12-103-0027	30119	n/a	6	1,100	Good	Deployed
n/a	Agilaire 8872	data logger	12-103-0027	0311	8/27/2014	6.5	6,600	Good	Deployed
n/a	Met One E-BAM Plus	PM 10	12-103-3004	X19175	9/17/2018	2.6	8,310	Good	Deployed
n/a	T-API T400	Ozone	12-103-5002	6022	9/30/2020	0.3	8,600	Good	Deployed
n/a	TEI 1405	PM 2.5	12-103-5002	1405A235701603	4/20/2016	4.8	13,000	Good	Deployed
n/a	RM Young 5305	Wind sensor	12-103-5002	12	n/a	5	1,100	Good	Deployed
n/a	Agilaire 8872	data logger	12-103-5002	0312	8/27/2014	6.5	6,600	Good	Deployed
n/a	T-API 703E	O ₃ Primary	12-103-5002	331	5/14/2014	6.8	10,000	Good	Deployed
n/a	Topline Building, Inc.	Building	12-103-5002	n/a	12/20/2002	18.4	10,422	Fair	Deployed
n/a	Aluma Tower 10m	wind tower	12-103-5002	na	4/18/1997	24.1	2,000	Fair	Deployed
n/a	Envirronics 7000	Zero Air	12-103-5003	8639	9/17/2019	1.6	4,700	Good	Deployed
n/a	TEI 43i	SO ₂	12-103-5003	1170120019	12/14/2016	4.2	12,500	Good	Deployed
n/a	Agilaire 8872	data logger	12-103-5003	0608	12/9/2016	4.2	7,380	Good	Deployed
n/a	Envirronics 6100	Calibrator	12-103-5003	6186	8/1/2014	6.8	8,800	Good	Deployed
n/a	n/a	Building	12-103-5003	n/a	9/18/1987	33.6	4,850	Fair	Deployed
n/a	TEI 42i	NOx	Broward Co.	CM08260023	7/24/2008	12.8	11,000	Fair	Spare
n/a	Advance	Building	n/a	n/a	7/26/1989	31.8	5,000	Fair	Spare
n/a	T-API T640	PM 2.5	Office	566	11/29/2018	2.4	21,000	Good	Spare
n/a	Envirronics 6100	Calibrator	Office	7866	4/2/2018	3.1	9,000	Good	Spare
n/a	TEI 42i	NOx	Office	11636300019	12/14/2016	4.2	14,500	Good	Spare
n/a	T-API T300	CO	Office	2425	5/4/2016	4.8	10,800	Good	Spare
n/a	RM Young 5305	Wind sensor	Office	80703	9/25/2015	5.6	1,100	Good	Spare
n/a	Agilaire 8872	data logger	Office	0307	8/27/2014	6.5	6,600	Good	Spare
n/a	Agilaire 8872	data logger	Office	0308	8/27/2014	6.5	6,600	Good	Spare
n/a	T-API 703E	O ₃ Primary	Office	332	5/14/2014	6.8	10,000	Good	Spare
n/a	RM Young 5305	Wind sensor	Office	69489	n/a	7	1,100	Good	Spare
n/a	T-API T400	Ozone	Office	85	n/a	9	n/a	Good	Spare
n/a	T-API 400E	Ozone	Office	2545	8/17/2010	10.5	7,200	Good	Spare
n/a	T-API 400E	Ozone	Office	2560	8/17/2010	10.5	7,200	Good	Spare
n/a	T-API 703E	O ₃ Primary	Office	240	8/6/2009	11.5	9,000	Good	Spare
n/a	TEI 49i	Ozone	Office	CM08270005	8/6/2009	11.8	9,000	Good	Spare
n/a	TEI FRM 2025	PM2.5 FRM	Office	2025B222800806	9/19/2008	12.6	12,406	Fair	Spare
n/a	Envirronics 6100	Calibrator	Office	3942	4/24/2007	14.0	8,900	Good	Spare
n/a	Envirronics 6103	Calibrator	Office	2818	3/25/2002	19.1	10,600	Good	Spare
n/a	ESC 8816	data logger	Office	4406	4/12/2002	19	3,900	Fair	Spare
n/a	ESC 8816	data logger	Office	4407	4/12/2002	19	3,900	Fair	Spare
n/a	ESC 8816	data logger	Office	4408	4/12/2002	19	3,900	Fair	Spare
n/a	ESC 8816	data logger	Office	4409	4/12/2002	19	3,900	Fair	Spare
n/a	ESC 8816	data logger	Office	4410	4/12/2002	19	3,900	Fair	Spare
n/a	TEI 43C	SO ₂	Office	43C-55928-305	6/26/1996	24.7	6,500	Fair	Spare

Broward County EEPD									
Property /Identification No.	Manufacturer and Model No.	Description	Location	Serial No.	Acquisition Date	Age	Initial Cost	Condition	Status
308795	ESC 8832	Data Logger	12-011-0033	A3855K	9/25/12	8.4	\$6,350.00	Good	active
NONE	Met One RAM-1020 with VSCL	Non-FEM PM2.5 Continuous Monitor	12-011-0033	P16733	8/19/13	7.5	\$16,633.00	Good	active
NONE	RM Young Wind Speed/Wind Dir	WS/WD	12-011-0033	146400	1/30/07	14.1	\$2,008.17	Good	active
NONE	RM Young T/RH Sensor	T/RH	12-011-0033	2047	12/19/11	9.2	\$1,061.50	Good	active
310340	Thermo 49i	O3 Analyzer	12-011-0033	113748257	5/17/11	9.8	\$8,112.00	Good	active
310341	Thermo 49i-PS	O3 Calibrator	12-011-0033	113748258	5/17/11	9.8	\$11,194.00	Good	active
308796	ESC 8832	Datalogger	12-011-0034	A3856K	9/25/12	8.4	\$6,350.00	Good	active
NONE	ESC 8832	Data Logger	12-011-0034	2372	6/1/12	8.7	\$7,920.00	Good	active
NONE	ATEC 2200	VOC Sampler	12-011-0034	37538	4/6/17	3.9	\$13,650.00	Good	active
NONE	RM Young Wind Speed/Wind Dir	WS/WD	12-011-0034	T75954	6/1/12	8.7	\$1,642.00	Good	active
NONE	RM Young T/RH Sensor	T/RH	12-011-0034	2047	12/19/11	9.2	\$1,061.50	Good	active
NONE	URG	CSN Network URG Monitor	12-011-0034	08580	1/10/8	13.1	paid by EPA	Good	active
NONE	SuperSASS	CSN Network SuperSASS Monitor	12-011-0034	N9188	6/22/12	8.7	\$13,695.50	Good	active
NONE	Teledyne 701H	HP Zero Air	12-011-0034	284	2/7/12	9.0	\$6,971.70	Good	active
NONE	Teledyne 7700U	Dilution Calibrator	12-011-0034	635	3/20/20	0.9	\$23,351.50	NEW	active
NONE	Thermo 2025i	PM2.5 Manual Sampler (1-in-3)	12-011-0034	20451	9/16/13	7.4	\$13,967.85	Good	active
NONE	Teledyne T640X	T640X	12-011-0034	663	4/10/19	1.9	\$36,532.00	Good	active
322918	Thermo 42i-LY	NO/NO/NODiff	12-011-0034	1202549016	9/8/20	0.4	\$32,330.54	Good	active
NONE	Thermo 44i-TLE	SO2 TL	12-011-0034	1171790011	8/1/17	3.5	\$16,946.77	Good	active
285684	Thermo 48C-TLE	COTL	12-011-0034	05105711728	9/22/05	15.4	\$11,655.02	Good	active
N/A	Thermo 49i	O3 Analyzer	12-011-0034	1308589757	8/1/20	0.5	LOANER	Good	Loaned from Thermo
296246	Thermo 49i-PS	O3 Calibrator (spare)	12-011-0034	727625035	9/21/07	13.4	\$10,812.50	Good	to be sent for annual O3 certification
296246	Thermo 49i-PS	O3 Calibrator	12-011-8002	1150770008	3/2/15	6.0	\$13,333.51	Good	active
310131	Tisch TE-6070V	PM10 Manual Sampler Collocated (1-in-6)	12-011-0034	1783	1/20/11	10.1	\$6,366.00	Good	inactive
310130	Tisch TE-6070V	PM10 Manual Sampler Primary (1-in-6)	12-011-0034	2231	8/2/12	8.5	\$7,368.00	Good	inactive
NONE	Thermo 2025i	PM2.5 Manual Sampler Primary (1-in-3)	12-011-0034	20450	9/16/13	7.4	\$14,373.50	Good	Not working - lightning
311329	Thermo 2025i	PM2.5 Manual Sampler Collocated (1-in-12)	12-011-0034	20262	8/17/12	8.5	\$14,373.50	Good	inactive
Built by CAS as one turn-key unit. GC FID is Chromatoc, M41022									
NONE	CAS Auto GCF-ID	12-011-0034	596308020		12/7/20	0.2	EPA PAID + \$13,122.43 (enclosure with AC)	New	PAMS
NONE	ESC 8872	Data Logger	12-011-0034	979	1/27/20	1.1	\$8,750.00	NEW	PAMS
NONE	ATEC 8000-2	Carbonyl Sampler	12-011-0034	TBD	TBD		\$17,470.00	New	PAMS
NONE	Vaisala CL-51	Celometer	12-011-0034	TBD	BD		\$34,387.37	New	PAMS
NONE	Kipp & Zonen SMP6-V	Solar Radiation	12-011-0034	190468	1/4/21	0.1	\$2,212.50	New	PAMS
NONE	Kipp & Zonen SLU5-V	UV Radiation	12-011-0034	201054	1/4/21	0.1	\$3,288.00	New	PAMS
NONE	RM Young 52203	Rain Tipping Bucket	12-011-0034	TB16047	7/21/20	0.6	\$592.50	New	PAMS
NONE	RM Young 41342VC	Pt Temp	12-011-0034	T532664	7/21/20	0.6	\$512.00	New	PAMS
NONE	RM Young 61402V	Barometric Pressure	12-011-0034	BPA14705	7/21/20	0.6	\$983.00	New	PAMS
NONE	Teledyne API T500U	Direct Measure NO2	12-011-0034	311	9/1/20	0.5	\$17,100.00	New	PAMS
NONE	ESC 8832	Data Logger	12-011-0035	A4462K	8/9/13	7.5	\$7,910.00	Good	active
311540	Teledyne 633	Aethalometer	12-011-0035	AE33-501-00115	5/17/12	8.8	\$21,997.00	Good	active
NONE	Teledyne T200UP	Analyzer: NO-NO2 (Trace, Photolytic)	12-011-0035	141	7/29/19	1.6	\$18,415.00	Good	active
NONE	Teledyne 701H	HP Zero Air	12-011-0035	441	12/31/18	2.1	\$7,340.00	Good	active
311541	Teledyne 7700U	Dilution Calibrator	12-011-0035	85	5/14/15	5.8	\$20,888.10	Good	active
311542	Thermo 48i-TLE	CO TL	12-011-0035	829	1/23/20	1.1	\$24,394.00	Good	active
NONE	TSI UFP3031	Continuous Particulates Ultrafine	12-011-0035	3301202404/3031120501	10/3/12	8.4	\$61,295.00	Good	active
311501	ESC 8832	Data Logger	12-011-2003	A4206K	9/25/12	8.4	\$6,350.00	Good	active
paid by EPA	R. M. Young 81000	Sonic Anemometer	Env. Monitoring Lab	3485	9/1/10	10.5	paid by EPA	Good	Communication issues - inactive
NONE	RM Young Wind Speed/Wind Dir	WS/WD	12-011-2003	154837	5/31/17	3.7	\$14,626.00	Good	active
296245	Thermo 49i	O3 Analyzer	12-011-2003	CM07340004	9/24/07	13.4	\$7,681.50	Good	active
296244	Thermo 49i-PS	O3 Calibrator	12-011-2003	727625034	9/21/07	13.4	\$10,812.50	Good	active
NONE	Teledyne T640	PM2.5 Continuous Monitor	12-011-2003	448	9/1/18	2.5	\$23,447.00	Good	active
310232	Thermo Partisol Plus 2025	PM2.5 Manual Sampler (1-in-3)	12-011-2003	22735	6/2/13	7.7	\$13,637.80	Good	inactive
NONE	Thermo Partisol Plus 2025	PM2.5 Manual Sampler (1-in-3)	12-011-2003	22704	3/18/11	9.9	\$12,900.00	Poor	SURPLUS - waiting for approval
NONE	MetOne E-BAMS Plus	Continuous PM10	12-011-2003	W20762	10/4/17	3.4	\$10,457.70	REPAIRED	Back-up for Site 30 E-BAM Plus
donated	ESC 8832	Data Logger	12-011-5005	A0603	3/24/16	4.1	donated FDEP	Good	active
NONE	Teledyne T640	PM2.5 Continuous Monitor	12-011-5005	662	9/1/18	2.5	\$29,455.00	Good	active
331532	MetOne E-BAMS Plus	Continuous PM10	12-011-5005	W20769	10/4/17	3.4	\$10,457.70	Good	active
NONE	Thermo 2025i	PM2.5 Manual Sampler (Daily)	12-011-5005	20760	3/2/15	6.0	\$15,869.97	Good	inactive
311500	ESC 8832	Data Logger	12-011-8002	A4205K	9/25/12	8.4	\$6,350.00	Good	active
NONE	Teledyne 7700U	Dilution Calibrator	12-011-8002	513	7/29/19	1.6	\$22,780.00	Good	active
310908	Teledyne 701H	HP Zero Air (spare)	12-011-8002	536	5/14/15	5.8	\$5,932.50	Good	active
NONE	Thermo 42i	NO2/NO/NOx	12-011-8002	1170960054	5/8/17	3.8	\$18,032.82	Good	active
U of Mich. A555472	Thermo 49i	O3 Analyzer	12-011-8002	CM08320015	9/1/12	8.5	Donated	Good	active
NONE	Thermo 49i-PS	O3 Calibrator	12-011-8002	1172300029	9/19/17	3.4	\$16,357.31	Good	active
DONATED	ESC 8832	Data Logger	991Q	A4773K	3/24/16	4.1	donated FDEP	Good	active
NONE	Teledyne T400	O3 Analyzer	991Q	5931	6/1/20	0.7	\$9,702.50	NEW	TESTING
NONE	Thermo 49i	O3 Analyzer	991Q	CM09080404	4/8/09	11.9	\$7,533.50	Good	TESTING
donated	Thermo 49i-PS	O3 Calibrator	991Q	824931779	9/1/12	5.5	Donated	Good	Back-up
NONE	Thermo 49iQ	O3 Analyzer	991Q	1173380012	3/15/18	2.9	\$14,215.22	NEW	TESTING
NONE	Thermo 49iQ	O3 Analyzer	991Q	1173380011	3/15/18	2.9	\$14,215.22	NEW	At Thermo for repair
NONE	Thermo 49iQ	O3 Analyzer	991Q	1173380010	3/15/18	2.9	\$14,215.22	NEW	At Thermo for repair
NONE	Thermo 49iQ	O3 Analyzer	991Q	1173380013	3/15/18	2.9	\$14,215.22	NEW	TESTING
335213	Thermo 49i-PS	O3 Calibrator	991Q	1190651893	3/19/19	1.1	\$18,452.49	NEW	TESTING
NONE	Thermo 42i-TLE	NO/NO/NODiff	991Q	1171790012	8/21/17	3.4	\$32,736.72	Needs Repair	Needs motherboard and ozonator solenoid switch
NONE	Thermo 42i	NO2/NO/NOx	991Q	1163620012	10/1/16	4.4	\$17,700.47	Needs Repair	Back-up
322918	Thermo 42i-LY	NO/NO/NODiff	991Q	1160570008	9/8/16	4.4	\$28,243.09	Poor	Lightning
335219	Thermo 49i-PS	O3 Calibrator	Env. Monitoring Lab	1190651894	3/18/19	1.1	\$18,452.49	NEW	Needs O3 certification
NONE	Thermo 146iQ	Gas Calibrator	Env. Monitoring Lab	1172270037	5/1/19	1.0	\$23,479.55	NEW	TESTING
NONE	ATEC 2200	VOC Sampler	Env. Monitoring Lab	39650	7/31/19	1.6	\$10,095.00	NEW	TESTING
NONE	ATEC 2200	VOC Sampler	Env. Monitoring Lab	39648	7/31/19	1.6	\$10,095.00	NEW	TESTING
NONE	RM Young WindSpeed/Wind Dir	WS/WD	Env. Monitoring Lab	170143	7/11/19	1.6	\$1,561.25	NEW	Back-Up
NONE	RM Young WindSpeed/Wind Dir	WS/WD	Env. Monitoring Lab	170144	7/11/19	1.6	\$1,561.25	NEW	Back-Up
311327	Teledyne T200UP	Analyzer: NO-NO2 (Trace, Photolytic)	Env. Monitoring Lab	60	6/9/12	8.7	\$25,119.80	Good	MOCK UP SITE/Back-Up
NONE	Teledyne T640X	T640X	Env. Monitoring Lab	664	4/10/19	1.9	\$36,532.00	Good	MOCK UP SITE/Back-Up (repaired after Lightning)
NONE	Teledyne T640	PM2.5 Continuous Monitor	Env. Monitoring Lab	449	9/1/18	2.5	\$29,455.00	Good	MOCK UP SITE/Back-Up
NONE	Thermo 42i	NO2/NO/NOx	Env. Monitoring Lab	CM08260030	8/6/08	12.5	\$10,925.00	Good	Received back from Thermo (Repair) - need to test
NONE	Thermo 49i	Data Logger	Env. Monitoring Lab	M4296K	9/25/12	8.4	\$7,910.00	Good	inactive
NONE	Thermo 49i	Zero Air Generator	Env. Monitoring Lab	M569	5/22/17	3.7	\$7,210.00	Good	MOCK UP SITE/Back-Up
311647	Teledyne 701H	O3 Primary Standard	Env. Monitoring Lab	821	6/1/20	0.7	\$14,704.20	NEW	Needs O3 certification
310200	Teledyne 7700U	Dilution Calibrator	Env. Monitoring Lab	57	1/25/11	10.1	\$18,996.00	REPAIRED	MOCK UP SITE/Back-Up
NONE	Thermo 43i-TLE	SO2 TL	Env. Monitoring Lab	1428862875	10/10/14	6.4	\$13,377.58	Good	MOCK UP SITE/Back-Up
NONE	Thermo 48i-TLE	CO TL	Env. Monitoring Lab	1182480012	2/19/19	2.0	\$20,426.52	NEW	MOCK UP SITE/Back-Up
335212	Thermo 49i-PS	O3 Calibrator	Env. Monitoring Lab	1190651892	3/18/19	1.1	\$18,452.49	NEW	TESTING
NONE	R. M. Young 81000	Sonic Anemometer	Env. Monitoring Lab	1759	2/24/12	9.0	\$2,606.50	Good	For site 35
NONE	Teledyne T700U	Calibrator	Env. Monitoring Lab	387	5/22/17	3.7	\$22,987.90	Good	to FDEP (going to Site 8002)
Pinellas	Thermo 42i	NO2/NO/NOx	Env. Monitoring Lab	CM08260023	10/1/20	0.4	\$1,561.25	Good	Loaned from Pinellas
donated	ESC 8832	Datalogger	Env. Monitoring Lab	W279	3/24/16	4.9	\$1,561.25	Good	SURPLUS
NONE	Thermo 48i-TLE	CO TL	Env. Monitoring Lab	1170960053	5/11/17	3.8	\$15,616.24	Good	Needs repair - lightning strike
331533	MetOne E-BAMS Plus	Continuous PM10	STORAGE UNIT	W20770	10/4/17	3.4	\$10,157.70	Good	NOT WORKING
NONE	R&P TEOM 1400AB	Continuous PM2.5	STORAGE UNIT	1404B267250705	6/18/07	13.7	\$18,525.00	Good	SURPLUS
NONE	Teledyne T100	SO2 Analyzer	STORAGE UNIT	795	6/1/13	7.7	\$10,240.00	Poor	SURPLUS
DONATED	Teledyne T100	SO2 Analyzer	STORAGE UNIT	114	4/20/14	6.8	\$10,370.00	Good	SURPLUS
NONE	Teledyne T300	CO Analyzer	STORAGE UNIT	720	6/1/13	7.7	\$10,370.00	Good	To be donated to Miami
NONE	Thermo 5014i	PM2.5 Continuous Monitor	STORAGE UNIT	CM1491003	9/18/13	7.4	\$20,365.00	Poor	SURPLUS
NONE	Thermo 5014i	PM2.5 Continuous Monitor	STORAGE UNIT	CM1498101	11/5/14	6.3			

Agency Name Palm Beach County									
Property /Identification No.	Manufacturer and Model No.	Description	Location	Serial No.	Acquisition Date	Age	Initial Cost	Condition	Status
F01796000000000	Hitachi	OSCILLOSCOPE,TRANSCAT MDL 8578	HQ	7092874	09-Dec-87	33	\$1,005.48 3	Surplussed	
F07265000000000	Andersen Sampler, Inc	AIR SAMPLER,MDL.PM-10	BG	68-13	28-Apr-89	31	\$2,858.95 3	Surplussed	
F07435000000000	Andersen Sampler, Inc	SAUV-16H HIGH VOLUME AIR SAMPL (HEAD)	BG	10-16	17-May-89	31	\$2,858.75 3	Surplussed	
G01788000000000	Tisch Environmental, Inc	SAMPLER SYSTEM, PUF GPS-1	BG	13905	22-Jan-91	29	\$1,925.00 3		
G09062000000000	Entech Instrument	ORG.COMPOUND CANISTER 87-200	RBWH	391-265	04-Apr-91	29	\$6,825.00 4		
J03566000000000	Thermo Environmental	ZERO AIR SUPPLY III	HQ	111-34508-248	13-Sep-91	29	\$2,783.50 3		
J03600000000000	Wells Cargo	TRAILER,WELLS CARGO MDL EW1211	TMB	022776	16-Mar-92	28	\$8,170.00 3	This trailer was towed to the warehouse. Surplussed?	
J08043000000000	Thermo Environmental	ZERO AIR SUPPLY MDL 111	HQ	111-34901-248	10-Oct-91	29	\$2,783.50 3		
J08312000000000	Thermo Environmental	MULTIGAS CALIBRATOR MDL 146	RBWH	146T-36529-253	05-Feb-92	28	\$8,392.14 3	Old and obsolete	
K02660000000000	Bios International	CALIBRATOR KIT W/CELL&PRINTER	HQ	84702001144	07-Apr-93	27	\$2,321.15 3	Dry Cal flow standard	
10134428000000	Wells Cargo	2001 TRAILER, WELL CARGO UTIL	RPB	1WC200H2513 047441	01-Oct-01	19	\$11,690.35 3	2001 TRAILER, WELL CARGO UTIL RESCUECHAIR, #1900, Part of Toxic Air sampler	
10134429000000	Entech Instrument, Inc.	WEEKLY TIMER MODULE	HQ	160	01-Oct-01	19	\$1,150.00 3	PC, DELL DESKTOP.	
10134468000000	Dell	PC, DELL DESKTOP	RPB	CC2Q211	19-Dec-01	19	\$1,675.00 3	10/13/2014-To be surplussed as soon as PC, DELL DESKTOP.	
10134469000000	Dell	PC, DELL DESKTOP	RBWH	8C2Q211	19-Dec-01	19	\$1,675.00 3	10/13/2014-To be surplussed as soon as	
10135009000000	BGI Inc	PUMP PZM-200 SAMPLING SYSTEM	HQ	1662	16-Oct-00	20	\$8,539.03 2	PUMP PZM-200 SAMPLING SYSTEM PM2.5 single sampler	
10135016000000	Sartorius	ANALYTICAL FILTER WEIGHT BALNC	HQ	12008133	28-Sep-00	20	\$4,459.00 3	ANALYTICAL FILTER WEIGHT BALNC	
10135055000000	Thermo Environmental	PHOTOMETRIC ANALYZER UB #49C	HQ	49G67037-354	24-Aug-00	20	\$7,875.00 3	PHOTOMETRIC ANALYZER UB #49C	
10135847000000	Thermo Environmental	THERMO ELECT CALIBRATOR 146-C	HQ	146C-61874-333	02-Oct-98	22	\$10,100.00 3	THERMO ELECT CALIBRATOR 146-C	
10135877000000	Thermo Environmental	TEC0111-001 ZERO AIR SUPPLY	HQ	11161759-333	02-Nov-98	22	\$3,990.00 2	TEC0111-001 ZERO AIR SUPPLY	
10135878000000	Thermo Environmental	TECO 111-001 ZERO AIR SUPPLY	HQ	11161757-333	02-Nov-98	22	\$3,990.00 3	In use In use. 10/13/2014: Removed from AG Holley	
10143759000000	Dell	PC, DELL GX240 OPTIPLEX	HQ	CQZVG11	20-May-02	18	\$1,196.60 2	In use. 10/13/2014: Removed from AG Holley	
10143766000000	Dell	PC, DELL GX240 OPTIPLEX MINITR	TMB	H77V611	20-May-02	18	\$1,196.80 2	In use. 9/10/2014: Unit was surplussed through IT	
10143866000000	Dell	(COMPUTER)-STATION MANAGER DATA LOGGER	RBWH	11VW321	23-Dec-02	18	\$1,950.00 3	Obsolete	
10143918000000	Thermo Environmental	SEQUENTIAL SAMPLER 2025	RPB	2025B-21580-0204	05-Feb-03	17	\$1,000.00 2	In Use, We use SN 21580	
10143935000000	Dell	LAPTOP, DELL TOUGHBOOK 34-P3	HQ	ZAKYA	28-Apr-03	17	\$2,405.00 2	Obsolete and Broken	
10153053000000	Dell	SERVER, EMC CENTRAL DATABASE	HQ	1GJ1L21	01-Oct-03	17	\$1,500.00 2	Obsolete 9/10/2014: The unit was surplussed through IT.	
10153076000000	Dell	LAPTOP, DELL INSPIRON 8500	Surplus	BBG3L31	24-Oct-03	17	\$4,122.00 2	Surplused	
10155333000000	Thermo Environmental	U.V. PHOTOMETRIC O3 CALIBRATOR, 49C-PS	RPB	S17511995	27-Jun-05	15	\$8,127.00 2	Old, not in use	
10155373000000	Thermo Environmental	CORRELATION CARBON MONOXIDE ANALYZER, GAS FILTER	HQ	335203744	08-Jan-04	16	\$8,559.00 2	Old, Not in use Old, In use, 10/13/2014: Removed from AG Holley when it was closed:WAD	
10155374000000	Thermo Environmental	OZONE UV PHOTOMETRIC ANALYZER	HQ	335103738	08-Jan-04	16	\$6,354.00 2		
10155375000000	Thermo Environmental	PULSED FLUORESCENCE AMBIENT SULFUR DIOXIDE ANALYZER	HQ	0335003719	08-Jan-04	16	\$8,460.00 2	Old, Not in use Approx 9/2014, Unit was surplussed.	
10161221000000	Agilaire	DATA LOGGER, ESC MODEL 8832 AMBIENT	HQ	A0633	27-Jun-05	15	\$5,280.00 2	In use 4/14/2013: Calibrate Datalogger. 1/3/2014 : Unit is still in use at 20 Mile	
10161222000000	Agilaire	DATA LOGGER, ESC MODEL 8832 AMBIENT	AGH	A1030	27-Jun-05	15	\$5,280.00 2	In use	
10161223000000	Agilaire	DATA LOGGER, ESC MODEL 8832 AMBIENT	HQ	A1028	27-Jun-05	15	\$5,280.00 2		
10161224000000	Agilaire	DATA LOGGER, ESC MODEL 8832 AMBIENT	HQ	A1031	27-Jun-05	15	\$5,280.00 2		

101612260000000	Thermo Environmental	TEC0111-001 ZERO AIR SUPPLY, Compressor/Pump	HQ	0517912030	27-Jun-05	15	\$2,970.00	2	in use, at TMB Part of same order PCN 10161226/10161227 At HQ after TMB was closed - WAD
101612270000000	Thermo Environmental	TEC0111-001 ZERO AIR SUPPLY	RPB		27-Jun-05	15	\$1,188.00	2	At Royal Palm Beach,Part of same order PCN 10161226/10161227
101612440000000	Thermo Environmental	PARTISOL PLUS PM 2.5	RPB	99-008806	02-Jan-07	13	\$12,840.00	2	In use, SN 21927
101612830000000	Thermo Environmental	49I UV PHOTOMETRIC OZONE ANALYZER	HQ	0601213850	16-Nov-05	15	\$6,673.50	2	In Lab
101612840000000	Thermo Environmental	42I CHEMILUMINESCENT NOX ANALYZER	HQ	0601213919	16-Nov-05	15	\$9,733.50	2	NOT IN USE
101612860000000	Met One Instrument	MONITOR, BETA ATTENUATION W/POWER SUPPLY & ACCESSORIES	HQ	E5632	16-Nov-06	14	\$15,950.00	2	In the Lab for repair.
101641040000000	Agilair	AMBIENT DATA LOGGER ESC, MODEL 8832	BG	A1201	28-Nov-05	15	\$6,020.00	2	In use
101641050000000	Bios International Corp	LOW FLOW 5-500 SCCM	HQ	105982	30-Nov-05	15	\$4,000.00	2	Flow calibrator
101641060000000	Bios International Corp	HIGH FLOW 500-50,000	HQ	106379	30-Nov-05	15	\$4,000.00	2	Flow calibrator. 1/14/2014: Unit sent to MESA Laboratory for annual calibration.
101641080000000	Environics	MULTI-GAS CALIBRATION SYSTEM	TMB	3702	06-Dec-05	15	\$8,415.00	2	Not In use
101641690000000	Environics	CALIBRATION SYSTEM 6100	HQ	3830	12-Sep-06	14	\$8,415.00	2	
101679750000000	Thermo Environmental	UV PHOTOMETRIC OZONE ANALYZER	RPB	0711721591	11-Apr-07	13	\$6,777.00	2	In use
101679900000000	Thermo Environmental	GAS FILTER CORELATION CO ANALYZER MEASUREMENT	HQ	0703320497	26-Jan-07	13	\$9,085.50	2	
101679960000000	Environics	CALIBRATION SYSTEM SERIES 6100	AGH	3885	04-Dec-06	14	\$8,415.00	2	In use
101679970000000	Teledyne/API	TELEDYNE-API MODEL 703E UV PHOTOMETRIC MONITOR	AGH	0058	31-Oct-06	14	\$8,550.00	2	In use. Receipt date Nov 6, 2011
101720050000000	Wells Cargo	TRAILER, ENCLOSED FOR ENVIRONMENTAL	AGH	1WC200H2543 051414	01-Oct-06	14	\$13,750.00	2	
101720170000000	Thermo Environmental	FILTER EXCHANGE MECHANISM REV A	HQ	07022802	27-Jun-07	13	\$1,471.00	2	This was a repair part and should not have had its own PCN
101723940000000	Met One Instrument	BETA ATTENUATION MASS MONITOR, BAM1020 2.3FEM	RPB	06214	01-Oct-07	13	\$21,970.00	2	In use. In trailer
101723950000000	Bios International Corp	DEFINER 220 HIGH FLOW; RANGE:300-30,000 SCCM	HQ	112349	30-Sep-07	13	\$2,000.00	2	In use
101723960000000	Thermo Environmental	SULFER DIOXIDE ANALYZER, 43I PULSED	HQ	CM07350001	08-Oct-07	13	\$9,775.50	2	Surplussed
101747340000000	Wells Cargo	EXPRESS WAGON 16', MODEL EW1622	BG	1WC200G2383 05845	03-Jun-08	12	\$5,625.00	2	Triler in Belle Glade
101747350000000	R. M. Young	ULTRASONIC ANEMOMETER,YOUNG 85000	Surplus	1349	01-May-08	12	\$1,460.00	2	Broken Beyon Repair - Damage by birds Approx 9/2014, Unit was surplussed.
101747360000000	R. M. Young	ULTRASONIC ANEMOMETER,YOUNG 85000	Surplus	1348	01-May-08	12	\$1,460.00	2	Broken Beyon Repair - Damage by birds Approx 9/2014, Unit was surplussed.
101747430000000	Thermo Environmental	PARTIED PLUS 2025 SEQUENLIAL AIR SAMPLER	DB	2025B2221502 805	16-Jun-08	12	\$12,464.95	2	On roof of Delray Beach building 11/5/2013: Received evaluation quote from TEI for repair...WAD
101747450000000	Thermo Environmental	421I CHEMILUMINE NO-NO2 NOX ANALYZER	HQ	0816130476	01-May-08	12	\$10,706.50	2	11/20/2013: Unit shipped to Thermo
101747580000000	Agilair	DATA SYSTEM CONTROLLER, AMBIENT ESC MODEL 8832	HQ	A2821K	29-Sep-08	12	\$6,865.00	2	May have been damaged in the power outage at AGH
101759250000000	Thermo Environmental	UV PHOTOMETRIC OZONE (03) PRIMARY SOURCE CALIBRATOR	HQ	0906335234	23-Feb-09	11	\$10,165.00	2	In lab for repair
101759260000000	Met One Instrument	BETA-ATTENUATION MASS MONITOR,POWER SUPPLY	BG	H8630	23-Feb-09	11	\$14,300.00	2	In use
101759340000000	Thermo Environmental	PHOTOMELRIC OZONE ANALYZER, 49I UV	HQ	0908635705	06-Apr-09	11	\$7,533.50	2	10/15/2014....The front screen is illuminated but blank. Jason called TEI for help...wad. Determined that the 49i processor board was bad. Prepared quote

101825770000000	Dell	SERVER, DELL POWEREDGE T150	HQ	5969FN1	26-Aug-10	10	\$3,512.00	1	AirVision Database Computer, Computer is T110. The unit was sent to Agilaire in September
101826130000000	Met One Instrument	BETA ATTENUATION MASS MONITOR W/POWER	HQ	K18547	09-Dec-10	10	\$12,452.60	1	Running as PM10. Taken to HQ when AGH was closed - WAD
101826150000000	Dell	LAPTOP, DELL LATITUDE E6400 XFR	HQ	GJL8XL1	17-Nov-10	10	\$4,431.00	1	In use in use at AGH. Removed to HQ when AGH was closed...WAD
101871770000000	Teledyne/API	NOX ANALYZER	HQ	205	02-Dec-11	9	\$10,695.00	1	10/10/13: Unit moved from AGH to HQ. 12/16/13: PO approved for repair evaluation; awaiting RMA number from envirionics to sent the units in.
101887320000000	Environics	OZONE TRANSFER STANDARD SERIES 6103	HQ	4595	13-Nov-09	11	\$7,824.00	1	Needs repair. 12/16/13: PO approved for repair evaluation; awaiting RMA number from envirionics to sent the units in.
101887330000000	Environics	OZONE TRANSFER STANDARD SERIES 6103	HQ	4594	13-Nov-09	11	\$7,824.00	1	Needs repair. 12/16/13: PO approved for repair evaluation; awaiting RMA number from envirionics to sent the units in.
101920710000000	Thermo Environmental	PARTISOL 2025i SEQUENTIAL AIR SMAPLER	HQ	2025i-2036671303	29-Apr-13	7	\$13,200.50	1	
	Teledyne/API	OZONE TRANSFER STANDARD 703U	LL	254	15-Aug-19	1	\$15,208.00	1	
102149970000000	Teledyne/API	PARTICULATE MATTER ANALYSER 640X	HQ	807	8/15/2019	1	\$37,763.00	1	IN USE
	Agilaire	DATA SYSTEM CONTROLLER, AMBIENT ESC MODEL 8872	LL						
	Agilaire	DATA SYSTEM CONTROLLER, AMBIENT ESC MODEL 8872	DB		2/5/2020		\$9,135.00	1	IN USE
	Agilaire	DATA SYSTEM CONTROLLER, AMBIENT ESC MODEL 8872	LP		2/5/2020		\$9,135.00	1	IN USE

Orange County Environmental Protection Division									
Property /Identification No.	Manufacturer and Model No.	Description	Location	Serial No.	Acquisition Date	Age	Initial Cost	Condition	Status
764206	THERMO SCIENTIFIC 49I	OZONE ANALYZER	Winter Park	1170050010	2017/03/24	4	9492.27	Good	Active
764207	THERMO SCIENTIFIC 49I	OZONE ANALYZER	Skyview	1170050011	2017/03/24	4	9492.27	Good	Active
750204	THERMO SCIENTIFIC 49I	OZONE ANALYZER	Winter Park	1326659026	2013/09/30	7	9506.00	Good	Backup
770249	THERMO SCIENTIFIC 49IQ-ACNN	OZONE ANALYZER	Air Lab	1181340030	2018/09/24	2	12156.49	Good	Inactive
772120	THERMO SCIENTIFIC 49IQ	OZONE ANALYZER	Winter Park	1190180048	2019/05/24	1	10899.45	Good	Inactive
772122	THERMO SCIENTIFIC 49IQ	OZONE ANALYZER	Winter Park	1190180049	2019/05/24	1	10899.45	Good	Inactive
764204	THERMO SCIENTIFIC 48I	CO ANALYZER	Winter Park	1170050008	2017/03/24	4	13226.52	Good	Active
764205	THERMO SCIENTIFIC 48I	CO ANALYZER	Winter Park	1170050009	2017/03/24	4	13226.52	Good	Backup
755736	THERMO SCIENTIFIC 48I	CO ANALYZER	Winter Park	1500163900	2015/02/24	6	13472.82	Good	Backup
755737	THERMO SCIENTIFIC 48I	CO ANALYZER	Winter Park	1500163901	2015/02/24	6	13472.82	Good	Backup
766204	THERMO SCIENTIFIC 42I	NO2 ANALYZER	Winter Park	1172550002	2017/10/17	3	15406.41	Good	Active
755738	THERMO SCIENTIFIC 42I	NO2 ANALYZER	Winter Park	1500163902	2015/02/24	6	13927.68	Good	Backup
741524	THERMO SCIENTIFIC 42I	NO2 ANALYZER	Winter Park	1106147374	2011/02/24	10	11467.00	Good	Backup
772119	THERMO SCIENTIFIC 42IQ	NO2 ANALYZER	Winter Park	1190180051	2019/05/24	1	16045.86	Good	Inactive
770250	THERMO SCIENTIFIC 42IQ ACANB NO	NO2 ANALYZER	Air Lab	1181340031	2018/09/24	2	21973.45	Good	Inactive
751896	THERMO SCIENTIFIC 42I	NO2 ANALYZER	Winter Park	1336460152	2014/01/28	7	13754.88	Good	Backup
750205	THERMO SCIENTIFIC 43I	SO2 ANALYZER	Winter Park	JC1320600867	2013/09/30	7	11840.00	Good	Backup
766205	THERMO SCIENTIFIC 43I	SO2 ANALYZER	Winter Park	1172550003	2017/10/17	3	13346.85	Good	Active
755740	THERMO SCIENTIFIC 111	ZERO AIR GENERATOR	Winter Park	1500163903	2015/02/24	6	5519.00	Good	Backup
772123	THERMO SCIENTIFIC 111IQ	ZERO AIR GENERATOR	Winter Park	1182130025	2019/05/24	1	6295.03	Good	Active
766092	THERMO SCIENTIFIC 146IQ	GAS BLENDER	Winter Park	1172270023	2018/08/01	2	16612.71	Good	Inactive
747329	THERMO SCIENTIFIC 146I	GAS BLENDER	Winter Park	1227254853	2012/10/16	8	12900.89	Good	Active
755739	THERMO SCIENTIFIC 146I	GAS BLENDER	Winter Park	1500163897	2015/02/24	6	12871.00	Good	Backup
772121	THERMO SCIENTIFIC 146IQ	GAS BLENDER	Winter Park	1190180050	2019/05/24	1	16612.71	Good	Inactive
749643	THERMO SCIENTIFIC 49IPS	OZONE PRIMARY STANDARD	Winter Park	1336460151	2014/02/05	7	11779.60	Good	Active
764208	THERMO SCIENTIFIC 49I-PS	OZONE PRIMARY STANDARD	Skyview	1170050012	2017/03/24	4	13112.15	Good	Active
756626	THERMO SCIENTIFIC 49I-PS	OZONE PRIMARY STANDARD	Winter Park	1151380003	2015/07/07	5	12485.20	Good	Backup
750381	THERMO SCIENTIFIC 5014I	PARTICULATE ANALYZER	Winter Park	CM13351002	2013/10/04	7	21225.00	Good	Backup
755027	THERMO SCIENTIFIC 5014I	PARTICULATE ANALYZER	Winter Park	CM14291007	2014/10/22	6	18223.23	Good	Active
755028	THERMO SCIENTIFIC 5014I	PARTICULATE ANALYZER	Winter Park	CM14291008	2014/10/22	6	18223.22	Good	Active
762294	THERMO SCIENTIFIC 5014I	PARTICULATE ANALYZER	Winter Park	CM16131005	2016/09/21	4	18893.76	Good	Backup
761065	AGILAIRE 8872	DATA LOGGER	Winter Park	0550	2016/04/27	5	8085.00	Good	Active
761066	AGILAIRE 8872	DATA LOGGER	Air Lab	0551	2016/04/27	5	8085.00	Good	Backup
761067	AGILAIRE 8872	DATA LOGGER	Skyview	0548	2016/04/27	5	8085.00	Good	Active
761068	AGILAIRE 8872	DATA LOGGER	Air Lab	0549	2016/04/27	5	8085.00	Good	Backup
756328	NOVALYNX 230-M202	BAROMETER	Skyview	1616000021	2016/07/28	4	1620.09	Good	Active
756329	NOVALYNX 230-M202	BAROMETER	Skyview	1616000018	2016/07/28	4	1620.10	Good	Backup
756330	NOVALYNX 230-M202	BAROMETER	Winter Park	1616000019	2016/07/28	4	1620.10	Good	Active
756331	NOVALYNX 230-M202	BAROMETER	Winter Park	1616000020	2016/07/28	4	1620.10	Good	Backup
755247	BIOS DEFINER 220-L	FLOW METER	Winter Park	141461	2015/05/06	5	2045.60	Good	Backup
730582	BIOS DEFINER 220	FLOW METER	Winter Park	111132	2007/07/25	13	2010.00	Good	Backup
755246	BIOS DEFENDER 530-H	FLOW METER	FDEP QASL (recertification)	139494	2015/05/06	5	1743.40	Good	Recent in Progress
756338	BIOS DEFENDER 530-H	FLOW METER	Winter Park	137288	2015/01/16	6	1750.00	Good	Backup
755697	CHINOOK STREAMLINE PRO MODEL M	FLOW METER	Winter Park	C150101	2015/02/26	6	3137.24	Good	Backup
755698	CHINOOK STREAMLINE PRO MODEL S	FLOW METER	Winter Park	C150102	2015/02/26	6	3137.24	Good	Backup
N/A	VAISALA HM40	HYGROMETER	Winter Park	K4730049	2014/12/01	6	Good	Active	
N/A	VAISALA HM40	HYGROMETER	Winter Park	L1720058	2014/12/01	6	Good	Active	
N/A	CONTROL COMP DIGITAL THERMOMETER	DIGITAL THERMOMETER	Winter Park	L616301	N/A	N/A	N/A	Good	Active
N/A	CONTROL COMP DIGITAL THERMOMETER	DIGITAL THERMOMETER	Winter Park	130567028	N/A	N/A	N/A	Good	Active
N/A	CONTROL COMP DIGITAL THERMOMETER	DIGITAL THERMOMETER	Winter Park	61602143	N/A	N/A	N/A	Good	Active
N/A	CONTROL COMP DIGITAL THERMOMETER	DIGITAL THERMOMETER	Winter Park	101642099	N/A	N/A	N/A	Good	Active
753158	DELL OPTIPLEX 9020	COMPUTER	Main Office	BZXWL02	2014/07/25	6	734.05	Good	To be retired 2021
753160	DELL OPTIPLEX 9020	COMPUTER	Main Office	BZWWL02	2014/07/25	6	734.05	Good	To be retired 2021
755256	DELL OPTIPLEX 9020	COMPUTER	Main Office	DLN5T52	2015/09/17	5	651.33	Good	To be retired 2021
755363	DELL OPTIPLEX 9020	COMPUTER	Main Office	IJX8842	2015/03/02	6	1013.33	Good	To be retired 2021

755364	DELL OPTIPLEX 9020	COMPUTER	Winter Park	IJX7842	2015/03/02	6	1013.33	Good	To be retired 2021
755905	DELL OPTIPLEX 9020	COMPUTER	Skyview	FTP7B42	2015/04/21	6	1019.93	Good	To be retired 2021
755906	DELL OPTIPLEX 9020	COMPUTER	Skyview	FTQ6B42	2015/04/21	6	1019.93	Good	To be retired 2021
756467	DELL OPTIPLEX 9020	COMPUTER	Skyview	DLN7T52	2015/09/17	5	651.33	Good	To be retired 2021
755734	JUNIPER EX 2200 24T	ETHERNET SWITCH	Winter Park	CW02148215	2014/11/22	6	815.00	Good	Active
756546	JUNIPER EX2200	ETHERNET SWITCH	Air Lab	SCW02141914 82	2015/06/30	5	815.00	Good	Backup
756547	JUNIPER EX2200	ETHERNET SWITCH	Winter Park	SCW02141917 88	2015/06/30	5	815.00	Good	Backup
N/A	THERMO SCIENTIFIC N/A	FIRST STAGE INLET	Winter Park	10-10-2013-2B	2013/10/10	7	N/A	Good	Backup
N/A	THERMO SCIENTIFIC N/A	FIRST STAGE INLET	Winter Park	05-25-2014-1A	2014/05/25	6	N/A	Good	Backup
N/A	THERMO SCIENTIFIC N/A	FIRST STAGE INLET	Winter Park	10-10-2013-1A	2013/10/10	7	N/A	Good	Backup
N/A	THERMO SCIENTIFIC N/A	FIRST STAGE INLET	Winter Park	03-20-2013-1A	2013/03/20	8	N/A	Good	Backup
N/A	THERMO SCIENTIFIC N/A	FIRST STAGE INLET	Winter Park	10-10-2013-3C	2013/10/10	7	N/A	Good	Backup
757095	DELL LATITUDE E7450	LAPTOP	Winter Park	79W5762	2015/09/04	5	1105.32	Good	Active
746356	PANASONIC TOUGHBOOK 19	LAPTOP	Winter Park	2FKYA57981	2012/08/20	8	2600.00	Good	Backup
756664	VIZIO 55" FLAT SCREEN	MONITOR	Winter Park	LWZ2PPAQ38 02232	2015/06/24	5	3675.00	Good	Active
766454	THERMO SCIENTIFIC 60L	OVEN	Air Lab	42202295	2018/02/06	3	1141.49	Good	Backup
757682	LIEBERT GXT4-2000RT120	POWER BACKUP	Skyview	1510100421A FBB3	2015/07/01	5	1425.00	Good	Active
757230	LIEBERT GXT4	POWER BACKUP	Winter Park	1512900408A FBA3	2015/08/26	5	1100.00	Good	Active
762326	LIEBERT GXT4	POWER BACKUP	Winter Park	1626200335A FBA3	2017/03/28	4	1085.00	Good	Active
762327	LIEBERT GXT4	POWER BACKUP	Winter Park	1626200343A FBA3	2017/03/28	4	1085.00	Good	Active
756638	BGI FRACTIONATOR	VSCC	Winter Park	070614-166	2015/08/12	5	1648.36	Good	Backup
756639	BGI FRACTIONATOR	VSCC	Winter Park	270711-31	2015/08/12	5	1648.36	Good	Backup
756640	BGI FRACTIONATOR	VSCC	Winter Park	180514-25	2015/08/12	5	1648.36	Good	Backup
N/A	BGI FRACTIONATOR	VSCC	Winter Park	221112-180	N/A	N/A	1648.36	Good	Backup
N/A	BGI FRACTIONATOR	VSCC	Winter Park	147526	N/A	N/A	1648.36	Good	Backup
N/A	BGI FRACTIONATOR	VSCC	Winter Park	138712	N/A	N/A	1648.36	Good	Backup
773594	DELL LATITUDE 5400	LAPTOP	Operator	GMEP10ZL057	1/10/2020	1	1,515.00	Good	Active
773589	DELL LATITUDE 5400	LAPTOP	Operator	GMEP10ZL061	1/10/2020	1	1,515.00	Good	Active
773590	DELL LATITUDE 5400	LAPTOP	Operator	GMEP10ZL053	1/10/2020	1	1,515.00	Good	Active
N/A	DELL LATITUDE 5400	LAPTOP	Operator	GMEP10ZL055	1/10/2020	1	1,515.00	Good	Active
N/A	HP PCL 6	LASER PRINTER	Winter Park	N/A	N/A	N/A	N/A	Fair	Inactive
N/A	ZYXEL PK5001Z	MODEM	Winter Park	S140Y1006663	N/A	N/A	N/A	Good	Active
N/A	CISCO ASA 5505	FIREWALL	Winter Park	JMX1824Z04	N/A	N/A	N/A	Good	Active
N/A	CISCO ASA 5505	FIREWALL	Skyview	N/A	N/A	N/A	N/A	Good	Active
N/A	SIERRA WIRELESS GX450	CELL MODEM	Skyview	N/A	5/9/2019	1	N/A	Good	Active
N/A	CISCO ASA 5505	FIREWALL	Air Lab	N/A	N/A	N/A	N/A	Good	Backup
N/A	CISCO ASA 5505	FIREWALL	Air Lab	N/A	N/A	N/A	N/A	Good	Backup
N/A	HB ELECTRONICS N/A	THERMOMETER	Winter Park	110252	3/15/2016	5	N/A	Good	Active
N/A	HB ELECTRONICS N/A	THERMOMETER	SkyView	111354	3/15/2016	5	N/A	Good	Active
N/A	HB ELECTRONICS N/A	THERMOMETER	FDEP QAS1	111626	3/15/2016	5	N/A	Good	Backup
N/A	HB ELECTRONICS N/A	THERMOMETER	FDEP QAS1	112713	3/15/2016	5	N/A	Good	Backup
N/A	HB ELECTRONICS N/A	THERMOMETER	FDEP QAS1	112050	3/15/2016	5	N/A	Good	Backup
N/A	Dwyer	MANOMETER	Winter Park	N50Z	1/26/2015	6	N/A	Good	Active
N/A	Dwyer	MANOMETER	Winter Park	N03AA0213007	1/26/2015	6	N/A	Good	Active
N/A	THERMO SCIENTIFIC	SONICATOR	Winter Park	1202404	N/A	N/A	N/A	Good	Active
N/A	Nikon Forestry Pro II Laser Rangefinder	Rangefinder	Winter Park		6/18/2020	0	446.95	Good	Active
	MesaLabs Flexcal	FLOW METER	Winter Park			121	6400	Good	Active

Miami-Dade County										
Property /Identification No.	Manufacturer and Model No.	Description	Location	Serial No.	Acquisition Date	Age	Initial Cost	Condition	Status	
ID Requested	Thermo 1405	PM Analyzer	Kendall	1405A242751901	2/15/2019	0	\$20,680.00	Good	Active	
655487	Thermo 1400A	PM Analyzer	Office	140AB24690307	7/18/2003	18	\$20,544.00	Good	Active	
655488	Thermo 1400A	PM Analyzer	Homestead Fire Station	140AB246910307	7/18/2003	18	\$20,544.00	Good	Active	
ID Requested	Thermo 2025i	PM2.5 Sampler	Miami Fire Station	2025i W20908 1509	9/17/2015	6	\$18,200.00	Good	Active	
808752	Teledyne 300E	CO Analyzer	Lab Annex	2231	9/29/2008	13	\$20,544.00	Good	Active	
828399	Thermo 43I	SO2 Analyzer	Pensuco	13059569685	2012	9	\$12,120.00	Good	Active	
847867	Thermo 49I	Ozone Analyzer	Perdue	1429063113	10/2/2014	7	\$8,260.00	Good	Active	
847984	Thermo 49I	Ozone Analyzer	Perdue	1429063114	10/9/2014	7	\$8,260.00	Good	Active	
821943	Thermo 49I-PS	Ozone Calibrator	Perdue	1106747387	2012	9	\$11,500.00	Good	Active	
828400	Thermo 49I-PS	Ozone Calibrator	Rosenstiel	1303256525	2012	9	\$11,500.00	Good	Active	
650571	Environics 6100	Calibrator	Office	2988	9/9/2002	19	\$9,800.00	Good	Active	
847518	Environics 6100	Calibrator	Pensuco	6149	6/12/2014	7	\$9,800.00	Good	Active	
850706	Environics 6100	Calibrator	Rosenstiel	6255	3/23/2015	6	\$9,800.00	Good	Active	
852468	ESC 8872	Data Logger	Perimeter Road	0480	2017	4	\$9,125.00	Good	Active	
854375	ESC 8872	Data Logger	Perdue	0582	2017	4	\$9,125.00	Good	Active	
857329	ESC 8872	Data Logger	Rosenstiel	0693	2017	4	\$9,125.00	Good	Active	
857331	ESC 8872	Data Logger	Lab Annex	0692	2017	4	\$9,125.00	Good	Active	
819570	Teledyne M701	Zero Air Generator	Lab Annex	3299	2012	9	N/A	Good	Active	
819574	Teledyne M701	Zero Air Generator	Pensuco	3295	2012	9	N/A	Good	Active	
819575	Teledyne M701	Zero Air Generator	Rosenstiel	3298	2012	9	N/A	Good	Active	
856743	Teledyne T200	NO2 Analyzer	Office	3574	2017	4	\$11,500.00	Good	Active	
847698	Teledyne T200	NO2 Analyzer	Rosenstiel	1550	9/3/2014	7	\$11,500.00	Good	Active	
841289	Teledyne T200UP	NO2 TL Monitor	Office	117	2018	3	\$24,700.00	Good	Active	
ID Requested	Teledyne API-T640X	PM2.5 & PM10 Analyzer	Office	213	2017	4	\$35,395.00	Good	Active	
841290	Teledyne API-T640X	PM2.5 & PM10 Analyzer	Miami Fire Station	287	2017	4	\$35,395.00	Good	Active	
854236	Teledyne T700U	Calibrator	Perimeter Road	257	7/31/2015	6	\$21,970.00	Good	Active	
853352	Teledyne T701H	Zero Air Generator	Perimeter Road	145	7/31/2015	6	\$7,850.00	Good	Active	
609076	737	Zero Air Generator	Office	2645	1/21/1999	22	N/A	Good	Inactive	
609076	737	Zero Air Generator	Office	2645	1/21/1999	22	N/A	Good	Inactive	
ID Requested	Thermo 1405	PM Analyzer	Office	1405A242551812	12/30/2018	3	\$20,680.00	Good	Inactive	
ID Requested	Thermo 1405	PM Analyzer	Office	1405A242751901	12/30/2018	3	\$20,680.00	Good	Inactive	
659433	Thermo 2025	PM2.5 Sampler	Office	2025B216240304	7/18/2003	18	N/A	Poor	Inactive	
655485	ESC 8816	Data Logger	Office	4948	7/14/2003	18	N/A	Good	Inactive	
640071	ESC 8816	Data Logger	Office	1585	3/1/2002	19	N/A	Good	Inactive	
640070	ESC 8816	Data Logger	Office	4442	3/1/2002	19	N/A	Good	Inactive	
640068	ESC 8816	Data Logger	Office	4440	3/1/2002	19	N/A	Good	Inactive	
640069	ESC 8816	Data Logger	Office	4441	3/1/2002	19	N/A	Good	Inactive	
640072	ESC 8816	Data Logger	Office	4444	3/1/2002	19	N/A	Good	Inactive	
640073	ESC 8816	Data Logger	Office	4445	3/1/2002	19	N/A	Good	Inactive	
640067	ESC 8816	Data Logger	Office	4439	3/1/2002	19	N/A	Good	Inactive	
655484	ESC 8816	Data Logger	Office	48C-60244-327	7/14/2003	18	N/A	Poor	Inactive	
640074	ESC 8816	Data Logger	Office	4437	3/1/2002	19	N/A	Poor	Inactive	
650647	ESC 8816	Data Logger	Office	0331002823	9/13/2002	19	N/A	Poor	Inactive	
650648	ESC 8816	Data Logger	Office	48C-62461-335/5	9/13/2002	19	N/A	Poor	Inactive	
828028	ESC 8832	Data Logger	Office	A4448K	2010	11	\$6,600.00	Good	Inactive	
828029	ESC 8832	Data Logger	Office	A4446K	2010	11	\$6,600.00	Good	Inactive	
828030	ESC 8832	Data Logger	Office	A4449K	2010	11	\$6,600.00	Good	Inactive	
527508	1200	PM10 Head	Office	2117	7/27/1993	28	N/A	Good	Inactive	
496260	1200	PM10 Head	Office	2747	5/10/1988	33	N/A	Good	Inactive	
496261	1200	PM10 Head	Office	2748	5/10/1988	33	N/A	Good	Inactive	
655489	Thermo 1400A	PM Analyzer	Office	140AB246890307	9/4/2009	12	\$20,544.00	Poor	Inactive	
661185	Thermo 2025i	PM2.5 Sampler	Office	2025B217240408	9/14/2004	17	N/A	Good	Inactive	
659434	Thermo 2025i	PM2.5 Sampler	Office	2025B216110301	7/18/2003	18	N/A	Poor	Inactive	
659435	Thermo 2025i	PM2.5 Sampler	Office	2025B216260304	7/18/2003	18	N/A	Poor	Inactive	
661184	Thermo 2025i	PM2.5 Sampler	Office	2025B217190408	7/18/2003	18	N/A	Poor	Inactive	
ID Requested	Thermo 2025i	PM2.5 Sampler	Office	2025B210901606	7/8/2016	5	\$18,200.00	Good	Inactive	
854398	Thermo 2025i	PM2.5 Sampler	Office	2025W210421605	9/17/2015	6	\$18,200.00	Good	Inactive	
848716	Thermo 2025i	PM2.5 Sampler	Office	2025B206811408	9/4/2014	7	\$18,200.00	Good	Inactive	
ID Requested	Thermo 2025i	PM2.5 Sampler	Office	2025W209101509	9/17/2015	6	\$18,200.00	Poor	Inactive	
808753	Teledyne 300E	CO Analyzer	Office	2233	9/29/2008	13	\$6,600.00	Good	Inactive	
808754	Teledyne 300E	CO Analyzer	Office	2234	9/29/2008	13	\$6,600.00	Good	Inactive	
658304	Thermo 42C	NO2 Analyzer	Office	0331002822	9/25/2003	18	N/A	Good	Inactive	
819196	Thermo 42I	NO2 Analyzer	Office	1007741317	2010	11	N/A	Good	Inactive	
818999	Thermo 42I	NO2 Analyzer	Office	CM10360071	2009	12	N/A	Good	Inactive	
811764	Thermo 42I	NO2 Analyzer	Office	CM08190013	9/29/2008	13	N/A	Good	Inactive	
661214	Thermo 43C	SO2 Analyzer	Office	0431709340	9/30/2004	17	N/A	Good	Inactive	
658302	Thermo 43C	SO2 Analyzer	Office	0333503279	9/25/2003	18	N/A	Good	Inactive	
850213	Thermo 43I	SO2 Analyzer	Pensuco	JB1423701318	11/13/2014	7	\$12,120.00	Good	Inactive	
661212	Thermo 48C	CO Analyzer	Office	0431709338	9/30/2004	17	N/A	Good	Inactive	
661213	Thermo 48C	CO Analyzer	Office	0431709339	9/30/2004	17	N/A	Good	Inactive	
659392	Thermo 49C	Ozone Analyzer	Office	032650000001331	9/25/2003	18	N/A	Good	Inactive	
650568	Thermo 49C	Ozone Analyzer	Office	49C-76048-381	10/1/2002	19	N/A	Good	Inactive	
650569	Thermo 49C	Ozone Analyzer	Office	0331002821	10/1/2002	19	N/A	Good	Inactive	
651906	Thermo 49C	Ozone Analyzer	Office	02155698-3	10/1/2002	19	N/A	Poor	Inactive	
604808	Thermo 49C PS	Ozone Calibrator	Office	2025B216240304	2/11/1998	23	N/A	Good	Inactive	
604809	Thermo 49C PS	Ozone Calibrator	Office	49CPS-60713-328	2/11/1998	23	N/A	Good	Inactive	
604810	Thermo 49C PS	Ozone Calibrator	Office	49CPS-60715-328	2/11/1998	23	N/A	Good	Inactive	
604807	Thermo 49C PS	Ozone Calibrator	Office	49PC60619327	2/11/1998	23	N/A	Poor	Inactive	
850212	Thermo 49I-PS	Ozone Calibrator	Office	1430063227	11/13/2014	7	\$11,500.00	Poor	Inactive	
853237	Thermo 49I-PS	Ozone Calibrator	Office	1152610015	9/17/2015	6	\$11,500.00	Good	Inactive	
853238	Thermo 49I-PS	Ozone Calibrator	Office	1152610016	9/17/2015	6	\$11,500.00	Good	Inactive	
847517	Environics 6100	Calibrator	Office	6150	6/12/2014	7	\$9,800.00	Good	Inactive	
847519	Environics 6100	Calibrator	Office	6148	6/12/2014	7	\$9,800.00	Good	Inactive	
658868	Environics 6100	Calibrator	Office	3177	9/23/2003	18	\$9,800.00	Good	Inactive	
658869	Environics 6100	Calibrator	Office	2987	9/9/2002	19	\$9,800.00	Good	Inactive	
650570	Environics 6100	Calibrator	Office	48C-62460-335/5	9/9/2002	19	\$9,800.00	Poor	Inactive	
533459	737	Zero Air Generator	Office	48C-60245-327	1/21/1999	22	N/A	Good	Inactive	
650640	737	Zero Air Generator	Office	2780	1/21/1999	22	N/A	Good	Inactive	
650641	737	Zero Air Generator	Office	2779	1/21/1999	22	N/A	Good	Inactive	
655486	ESC 8816	Data Logger	Office	4956	7/14/2003	18	N/A	Good	Inactive	
640075	ESC 8816	Data Logger	Office	898	3/1/2002	19	N/A	Good	Inactive	
854373	ESC 8872	Data Logger	Office	0580	2017	4	\$9,125.00	Good	Inactive	
854374	ESC 8872	Data Logger	Office	0581	2017	4	\$9,125.00	Good	Inactive	
852699	ESC 8872	Data Logger	Office	0507	9/30/2015	6	\$9,125.00	Good	Inactive	
852700	ESC 8872	Data Logger	Office	0508	9/30/2015	6	\$9,125.00	Good	Inactive	
852701	ESC 8872	Data Logger	Office	0509	9/30/2015	6	\$9,125.00	Good	Inactive	

847982	ESC 8872	Data Logger	Office	0318	10/9/2014	7	\$9,125.00	Good	Inactive
847983	ESC 8872	Data Logger	Office	0319	10/9/2014	7	\$9,125.00	Good	Inactive
857330	ESC 8872	Data Logger	Office	0691	2017	4	\$9,125.00	Good	Inactive
808751	Teledyne M300E	CO Analyzer	Office	9C4442	9/4/2009	12	N/A	Good	Inactive
808752	Teledyne M300E	CO Analyzer	Office	9C4443	9/4/2009	12	N/A	Good	Inactive
819571	Teledyne M701	Zero Air Generator	Office	3300	2012	9	N/A	Good	Inactive
819572	Teledyne M701	Zero Air Generator	Office	3297	2012	9	N/A	Good	Inactive
819573	Teledyne M701	Zero Air Generator	Office	3284	2012	9	N/A	Good	Inactive
ID Requested	Teledyne T200	NO2 Analyzer	Lab Annex	3785	2017	4	\$11,500.00	Good	Inactive
847699	Teledyne T200	NO2 Analyzer	Office	1551	9/3/2014	7	\$11,500.00	Poor	Inactive
853351	Teledyne T200UP	NO2 Trace Analyzer	Office	96	7/31/2015	6	\$24,700.00	Good	Inactive
822887	Teledyne T400	Ozone Analyzer	Office	101	2015	6	\$4,250.00	Poor	Inactive
ID Requested	Teledyne API T640	PM2.5 Analyzer	Office	539	9/25/2018	3	\$26,570.00	Good	Inactive
ID Requested	Teledyne API T640	PM2.5 & PM10 Analyzer	Office	213	1/15/2019	0	\$21,500.00	Good	Inactive
ID Requested	Teledyne API T640X	PM2.5 & PM10 Analyzer	Office	287	2018	3	\$35,395.00	Good	Inactive
ID Requested	Teledyne API T700	Dilution Calibrator	Office	4642	2019	1	\$13,271.50	New	Inactive
ID Requested	Teledyne API T700	Dilution Calibrator	Office	4644	2019	1	\$13,271.50	New	Inactive
ID Requested	Teledyne API T700	Dilution Calibrator	Office	4645	2019	1	\$13,271.50	New	Inactive
ID Requested	Teledyne API T700	Dilution Calibrator	Office	4643	2019	1	\$13,271.50	New	Inactive
ID Requested	Teledyne API T700	Dilution Calibrator	Rosenstiel	4640	2019	1	\$13,271.50	New	Active
ID Requested	Teledyne API T701	Zero Air System	Lab Annex	1756	2019	1	\$5,027.50	New	Active
ID Requested	Teledyne API T701	Zero Air System	Rosenstiel	1758	2019	1	\$5,027.50	New	Active
ID Requested	Teledyne API T701	Zero Air System	Pennsuco	1757	2019	1	\$5,027.50	New	Active
ID Requested	Teledyne API T701	Zero Air System	Office	1755	2019	1	\$5,027.50	New	Inactive
ID Requested	Teledyne API T701	Zero Air System	Office	1754	2019	1	\$5,027.50	New	Inactive
ID Requested	Teledyne API T701	Zero Air System	Office	1759	2019	1	\$5,027.50	New	Inactive
ID Requested	Teledyne API T300	Gas Filter Correlation CO Monitor	Office	4754	2019	1	\$11,408.50	New	Inactive
ID Requested	Teledyne API T300	Gas Filter Correlation CO Monitor	Office	4755	2019	1	\$11,408.50	New	Inactive
ID Requested	Teledyne API T640	PM Mass Monitor	Office	715	2019	1	\$23,727.00	New	Inactive
ID Requested	Teledyne API T701H	Zero Air System	Office	7079	2020	1	\$7,650.00	New	Inactive
ID Requested	Teledyne API T200	NO2 Analyzer	Office	702	2020	1	\$12,150.00	New	Inactive
ID Requested	Teledyne API T700U	NO2 Analyzer-Trace level	Office	7071	2020	1	\$24,843.25	New	Inactive
ID Requested	TEI 49IQ	O3 Analyzer	Office	1201717983	2020	1	\$11,560.00	New	Inactive
ID Requested	TEI 49IQ	O3 Analyzer	Office	1201717985	2020	1	\$11,560.00	New	Inactive
ID Requested	TEI 49IQ	O3 Analyzer	Office	1201717984	2020	1	\$11,560.00	New	Inactive
ID Requested	TEI 43IQ	SO2 Analyzer	Office	1201717986	2020	1	\$15,181.00	New	Inactive
ID Requested	TEI 43IQ	SO2 Analyzer	Pennsuco	1201717987	2020	1	\$15,181.00	New	Inactive
ID Requested	Teledyne API T640	PM2.5 Analyzer	Office	706	2020	1	\$31,024.00	New	Inactive
ID Requested	Thermo 2025i	PM2.5 Sampler	Office	2025jW215132010	2020	1	\$22,244.42	New	Inactive
ID Requested	Thermo 2025i	PM2.5 Sampler	Office	2025jW215142010	2020	1	\$22,244.42	New	Inactive

City of Jacksonville										
Property /Identification No.	Manufacturer and Model No.	Description	Location	Serial No.	Acquisition Date	Age	Initial Cost	Condition	Status	
186859	N/A	Air Compressor	Lab	N/A	2009	12	1225.17	Fair	Backup	
2002640	42i - Nox	Analyzer	Kooker Park	1170310010	N/A	N/A	N/A	Good	Active	
2002645	42i - Nox	Analyzer	Pepsi Place	1170310009	N/A	N/A	N/A	Good	Active	
188994	42i - Nox	Analyzer	Lab	0817630890	2010	11	11304.56	Fair	Backup	
195337	42i - Nox	Analyzer	Lab	1327059041	N/A	N/A	N/A	Good	Parts	
172824	43C - SO2	Analyzer	Lab	0421007303	N/A	N/A	N/A	Poor	Parts	
175613	43C - SO2	Analyzer	Lab	0436610194	N/A	N/A	N/A	Fair	Parts	
184697	43C - SO2	Analyzer	Lab	43C-75636-380	N/A	N/A	N/A	Fair	Parts	
2002641	43i - SO2	Analyzer	Kooker Park	1170310008	N/A	N/A	N/A	Good	Active	
180789	43i - SO2	Analyzer	Lab	611616471	2006	12	N/A	Good	Backup	
176660	43i - SO2	Analyzer	Lab	0520811801	N/A	N/A	N/A	Fair	Backup	
179549	43i - SO2	Analyzer	Lab	0600914730	N/A	N/A	N/A	Fair	Backup	
193321	43i - SO2	Analyzer	Lab	1225154501	2012	9	10967.50	Poor	Parts	
197214	43i - SO2	Analyzer	Lab	1436363426	2014	7	12457.00	Good	Backup	
2002637	43i - SO2	Analyzer	Lab	1170310006	N/A	N/A	N/A	Good	Active	
N/A	43i-SO2	Analyzer	Cedar Bay	1170310007	N/A	N/A	N/A	Good	Inactive	
167934	48C - CO	Analyzer	Lab	48C-67479-356	N/A	N/A	N/A	Good	Backup	
167932	48C - CO	Analyzer	Lab	48C-67941-356	N/A	N/A	N/A	Fair	Parts	
167935	48C - CO	Analyzer	Lab	48C-67941-359	2001	20	8559.00	Poor	Parts	
N/A	48C - CO trace	Analyzer	Lab	48CTL-67186-356	N/A	N/A	N/A	Fair	Parts	
195338	48i - CO	Analyzer	Pepsi Place	1308857434	2014	7	12467.00	Good	Active	
180679	48i - CO	Analyzer	Lab	0611616470	N/A	N/A	N/A	Fair	Parts	
193160	48i - CO	Analyzer	Lab	1216753230	N/A	N/A	N/A	Fair	Parts	
197215	48i - CO	Analyzer	Lab	1436363425	2014	7	12467.00	Poor	Backup	
199824	48i - CO	Analyzer	Lab	11606000006	2016	5	12785.75	Good	Backup	
2002638	48i - CO	Analyzer	Lab	1170310013	N/A	N/A	N/A	Good	Inactive	
N/A	48i - CO	Analyzer	Lab	1170310014	N/A	N/A	N/A	Good	Inactive	
174139	49C - O3	Analyzer	Lab	423707710	2004	17	6354.00	Fair	Parts	
174138	49C - O3	Analyzer	Lab	0423707712	2004	17	6354.00	Fair	Parts	
174133	49C - PS	Analyzer	Lab	0423707707	2004	17	8127.00	Fair	Parts	
N/A	49i - ozone	Analyzer	Lab	1170480025	N/A	N/A	N/A	Good	Active	
2002639	49i - ozone	Analyzer	Mayo	117310016	N/A	N/A	N/A	8702.90	Good	Active
197158	49i - ozone	Analyzer	Cisco Dr	1430863374	2015	6	9640.00	Good	Active	
180678	49i - ozone	Analyzer	Sheffield Elementry	0611616471	N/A	N/A	N/A	Good	Active	
186855	49i - ozone	Analyzer	Lab	CM09040077	2009	12	6978.40	Fair	Backup	
186856	49i - ozone	Analyzer	Lab	CM09040078	2009	12	6978.40	Fair	Parts	
186857	49i - PS ozone	Analyzer	Sheffield Elementry	0908935367	2009	12	9416.00	Good	Active	
186858	49i - PS ozone	Analyzer	Mayo	1170480025	N/A	N/A	N/A	Good	Active	
N/A	49i - PS ozone	Analyzer	Cisco Dr	0908935366	2009	12	9416.00	Good	Active	
N/A	49i - PS ozone	Analyzer	Lab	1430863375	2015	6	N/A	Good	Active	
138481	49i - PS ozone	Analyzer	Lab	1225154500	2012	6	11233.50	Fair	Backup	
106278	N/A	Balance	Lab	3411155	N/A	N/A	N/A	Poor	Obsolete	
195340	6100	Calibrator	Lab	5736	2008	13	N/A	Good	Active	
189416	6100	Calibrator	Lab	4776	2010	11	8775.00	Good	Active	
182786	6100	Calibrator	Pepsi Place	3887	N/A	N/A	N/A	Fair	Backup	
184538	6100	Calibrator	Lab	4306	N/A	N/A	N/A	Fair	Active	
189417	6100	Calibrator	Lab	4775	2010	11	8775.00	Fair	Backup	
197600	6100	Calibrator	Cedar Bay	6508	2015	6	8887.50	Fair	Backup	
182787	6100	Calibrator	Kooker Park	3886	N/A	N/A	N/A	Fair	Backup	
189416	6100	Calibrator	Lab	4776	2010	11	8775.00	Good	Backup	
2002229	6100	Calibrator	Pepsi Place	7585	2017	4	N/A	Good	Backup	
184536	6100	Calibrator	Lab	4312	N/A	N/A	N/A	Fair	Backup	
197599	6100	Calibrator	Lab	6509	2015	6	8887.50	Fair	Backup	
2002228	6100	Calibrator	Pepsi Place	7586	2017	4	N/A	Good	Active	
2002230	6100	Calibrator	Roselle & Copeland	7584	2017	4	N/A	Good	Backup	
187085	6100	Calibrator	Kooker Park	4491	2009	12	8775.00	Good	Active	
187084	6100	Calibrator	Lab	4490	2009	12	8775.00	Good	Backup	
172646	Computer	Computer	Kooker Park	KCBX2R7	N/A	N/A	N/A	Fair	Active	
172648	Computer	Computer	Mayo	KCTA57T	N/A	N/A	N/A	Fair	Active	
N/A	Computer	Computer	Ft. Caroline	4VGTVN1	N/A	N/A	N/A	Fair	Inactive	
167681	Computer - Dell 1400	Computer	Cubicle	N/A	N/A	N/A	N/A	Fair	Active	
184695	Computer - Dell Latitude D630	Computer	Pepsi Place	BPVYZF1	N/A	N/A	N/A	Fair	Active	
N/A	Computer - Dell OptiPlex	Computer	Cisco Dr	79NP1B1	N/A	N/A	N/A	Fair	Active	
172512	Computer - IBM	Computer	Cedar Bay	KCRZ00A	N/A	N/A	N/A	Fair	Active	
180783	Computer - Think Centre	Computer	Cubicle	LKKL5G	N/A	N/A	N/A	Fair	Active	
172575	Computer IBM	Computer	Lab	KCRR74F	N/A	N/A	N/A	Fair	Active	
N/A	Laptop - ThinkPad (Alvin)	Computer	Cubicle	R9-EBZK1	N/A	N/A	N/A	Fair	Active	
184695	Laptop - ThinkPad PPL	Computer	Pepsi Place	BPVYZF1	N/A	N/A	N/A	Fair	Active	
172513	Computer	Computer	Sheffield Elementry	KCRR91M	N/A	N/A	N/A	Fair	Active	
162147	Computer - Dell XPS R400	Computer	Cubicle	GDKR0	N/A	N/A	N/A	Fair	Active	
183820	8832	Data Logger	Lab	A1943	2004	17	N/A	Good	Inactive	

172529	8832	Data Logger	Lab	A0541	2004	17	N/A	Good	Inactive
N/A	8832	Data Logger	Lab	A0538	2004	17	N/A	Good	Inactive
171778	8832	Data Logger	Lab	A0543	2004	17	N/A	Good	Inactive
183819	8832	Data Logger	Lab	A1942	2004	17	N/A	Good	Inactive
172525	8832	Data Logger	Lab	A0547	2004	17	N/A	Good	Inactive
195341	8832	Data Logger	Lab	A4688K	2014	7	N/A	Good	Inactive
172516	8832	Data Logger	Lab	A0540	N/A	N/A	N/A	Fair	Parts
N/A	8832	Data Logger	Lab	A0542	N/A	N/A	N/A	Fair	Backup
172526	8832	Data Logger	Lab	A0544	N/A	N/A	N/A	Fair	Parts
172517	8832	Data Logger	Lab	A0545	N/A	N/A	N/A	Fair	Backup
172518	8832	Data Logger	Lab	A0546	N/A	N/A	N/A	Fair	Good
172528	8832	Data Logger	Lab	A0549	N/A	N/A	N/A	Fair	Good
172527	8832	Data Logger	Lab	A0548	N/A	N/A	N/A	Fair	Parts
172524	8832	Data Logger	Lab	A0587	N/A	N/A	N/A	Fair	Backup
189681	8832	Data Logger	Lab	A3937K	2004	17	N/A	Good	Inactive
189680	8832	Data Logger	Lab	A3936K	N/A	N/A	N/A	Good	Inactive
172522	8832	Data Logger	Lab	A0586	N/A	N/A	N/A	Good	Inactive
2007832	8872	Data Logger	Kooker Park	8872_0842	2018	3	7911.22	Good	Active
2007839	8872	Data Logger	Sheffield Elementry	8872_0850	2018	3	7911.22	Good	Active
2007838	8872	Data Logger	Cedar Bay	8872_0847	2018	3	7911.22	Good	Active
2007834	8872	Data Logger	Mandarin Rd	8872_0851	2018	3	7911.22	Good	Active
2007831	8872	Data Logger	Mayo	8872_0846	2018	3	7911.22	Good	Active
2007836	8872	Data Logger	Cisco Dr	8872_0849	2018	3	7911.22	Good	Active
2007833	8872	Data Logger	Pepsi Place	8872_0844	2018	3	7911.22	Good	Active
2007835	8872	Data Logger	Lab	8872_0848	2018	3	7911.22	Good	Backup
2007837	8872	Data Logger	Lab	8872_0845	2018	3	7911.22	Good	Backup
171778	Enclosure	Enclosure	Mandarin Rd	343G-10 (COJ# from inven)	N/A	N/A	N/A	Fair	Inactive
184118	Definer 220 H	flow standard	Lab	112786	N/A	N/A	N/A	Good	Backup
162935	Manometer	Manometer	Lab	11MNO2	N/A	N/A	N/A	Fair	Backup
195344	Met Sensor	Met Sensor	Pepsi Place	N/A	N/A	N/A	N/A	Fair	Active
195347	Met Tower	Met Tower	Pepsi Place	N/A	N/A	N/A	N/A	Fair	Active
N/A	ThinkVision Monitor	Monitor	Kooker Park	8894881	N/A	N/A	N/A	Fair	Backup
125742	Toxgard - CO Monitor	Monitor	Lab	N/A	N/A	N/A	N/A	Fair	Active
144535	Toxgard - CO Monitor	Monitor	Lab	N/A	N/A	N/A	N/A	Fair	Active
144537	Toxgard - CO Monitor	Monitor	Lab	N/A	N/A	N/A	N/A	Fair	Active
144536	Toxgard - CO Monitor	Monitor	Roselle & Copeland	N/A	N/A	N/A	N/A	Fair	Inactive
189418	O3 PS - 6103	O3 PS - 6103	Lab	4781	N/A	N/A	N/A	Fair	Backup
105038	Olfactometer	Olfactometer	File Room	N/A	N/A	N/A	N/A	Poor	Backup
105039	Olfactometer	Olfactometer	File Room	N/A	N/A	N/A	N/A	Poor	Backup
N/A	Opti Plex 780	Opti Plex 780	Lab	CCFVVN1	N/A	N/A	N/A	Fair	Active
167292	HP Laser Jet 2100	Printer	Lab	USGZ182467	N/A	N/A	N/A	Fair	Backup
164189	HP Laser Jet 2101	Printer	Lab	N/A	N/A	N/A	N/A	Fair	Backup
177084	HP Laser Jet 2430drn	Printer	Cubicle	N/A	N/A	N/A	N/A	Fair	Backup
195345	Computer Rack	Rack	Pepsi Place	N/A	N/A	N/A	N/A	Good	Active
195346	Computer Rack	Rack	Pepsi Place	N/A	N/A	N/A	N/A	Good	Active
183596	2025	Sampler	Lab	2025B219720706	N/A	N/A	N/A	Fair	Backup
197212	2025i	Sampler	Lab	2025i206831409	2014	7	16361.25	Good	Inactive
197213	2025i dup	Sampler	Sunny Acres	2025i206911409	2014	7	16361.25	Good	Backup
197211	2025i	Sampler	Sunny Acres	2025i206891409	2014	7	16361.25	Good	Active
197694	2025i	Sampler	Lab	2025iW207931504	2015	6	17050.77	Good	Active
197615	5014i	Sampler	Pepsi Place	CM14501004	2015	6	16880.00	Good	Inactive
195339	5014i	Sampler	Lab	CM13351001	2014	7	15213.66	Fair	Backup
N/A	TE 1400A	Sampler	Lab	140AB267240705	N/A	N/A	N/A	Fair	Parts
188469	TE 1400ab	Sampler	Lab	140AB275771001	N/A	N/A	N/A	Fair	Parts
N/A	TE rp 1400A	Sampler	Lab	140AB267570706	N/A	N/A	N/A	Fair	Parts
171776	TEOM 1400	Sampler	Lab	140AB245080303	N/A	N/A	N/A	Fair	Parts
171777	TEOM 1400AB	Sampler	Lab	140AB245050303	N/A	N/A	N/A	Good	Inactive
197614	TEOM 1405	Sampler	Sheffield Elementry	1405A230661501	2015	6	17075.00	Good	Active
199821	TEOM 1405	Sampler	Mayo	1405A235821603	2016	5	16890.13	Good	Active
197613	TEOM 1405	Sampler	Lab	1405A230821502	2015	6	17075.00	Good	Inactive
N/A	Thermo 1405	Sampler	Lab	1405A241581808	N/A	N/A	N/A	Good	Backup
199822	TEOM 1405	Sampler PM10	Kooker Park	1405A235831603	2016	5	16890.13	Good	Active
199823	TEOM 1405	Sampler PM2.5	Kooker Park	1405A236021603	2016	5	16890.13	Good	Active
N/A	CAS Cargo Container	Shelter	Kooker Park	N/A	2018	3	85852.38	Good	Active
171440	Sonic Anemometer	Sonic Anemometer	Lab	N/A	N/A	N/A	N/A	Poor	Parts
171441	Sonic Anemometer	Sonic Anemometer	Lab	N/A	N/A	N/A	N/A	Poor	Parts
171442	Sonic Anemometer	Sonic Anemometer	Lab	N/A	N/A	N/A	N/A	Poor	Parts
116737	Supply Cabinet - metal	Supply Cabinet - metal	Lab	N/A	N/A	N/A	N/A	Fair	Active
2010486	Teledyne	T640	Pepsi Place	681	2019	2	23987.00	Good	Active
N/A	Teledyne	T640X	Mandarin Rd	725	2019	2	37194.00	Good	Active
168912	Trailer	Trailer	Sheffield Elementry	N/A	N/A	N/A	N/A	Poor	Active
144808	Trailer	Trailer	Cedar Bay	N/A	1994	27	4643.20	Poor	Active
N/A	Trailer	Trailer	Mandarin Rd	N/A	N/A	N/A	N/A	Poor	Active
153455	Trailer	Trailer	Mayo	N/A	N/A	N/A	N/A	Poor	Active

Environmental Protection Commission of Hillsborough County

Property /Identification No.	Manufacturer and Model No.	Description	Location	Serial No.	Acquisition Date	Age	Initial Cost	Condition	Status
163503	Thermo 43i	Sulfur Dioxide Analyzer	Apollo Bch	1151660006	10/31/2015		\$ 11,905.40	Good	Active
172237	Thermo 1405	TEOM PM MONITOR	Apollo Bch	1405A241001803	4/9/2018		\$ 20,565.75	Good	Active
173298	Teledyne-API T701	Zero Air System	Apollo Bch	1250	7/31/2018		\$ 4,365.00	Good	Active
162036	Thermo 146i	DYNAMIC GAS CALIBRATOR	Apollo Bch	1150560040	3/11/2015		\$ 11,000.00	Good	Active
105560	Agilaire 8832	DATA LOGGER	Apollo Bch	A4032K	10/15/1997		\$ 2,250.00	Good	Active
	Tisch TE-1000	High Volume Sampler	CSX Railyard	VFC P7639	8/12/2010			Good	Active
	Tisch TE-1000	High Volume Sampler	CSX Railyard	VFC P7669	8/12/2010			Good	Active
131962	ESC 8816	DATA LOGGER	CSX Railyard	5025	11/13/2003		\$ 6,255.00	Good	Active
159672	Thermo 49i	Ozone Analyzer	Davis Island	1417062039	6/19/2014			Good	Active
159674	Thermo 43i	Sulfur Dioxide Analyzer	Davis Island	JC1411401168	5/20/2014		\$ 11,905.40	Good	Active
164239	Thermo 1405	TEOM PM MONITOR	Davis Island	1405A233691512	4/30/2016		\$ 19,162.26	Good	Active
	DIY	Zero Air System	Davis Island	NA				Good	Active
139231	Thermo 49i PS	Ozone Calibrator	Davis Island	0717722871	7/20/2007		\$ 9,583.68	Good	Active
162037	Thermo 146i	DYNAMIC GAS CALIBRATOR	Davis Island	1150560039	3/12/2015		\$ 13,000.00	Good	Active
105558	Agilaire 8832	DATA LOGGER	Davis Island	A3193K	10/15/1997		\$ 2,250.00	Good	Active
162635	Thermo 43i	Sulfur Dioxide Analyzer	East Bay	1151630005	6/30/2015		\$ 11,905.40	Good	Active
174874	Teledyne-API	Zero Air System	East Bay	481	1/1/2016	4	\$ 4,385.00	Good	Active
105566	Agilaire 8832	DATA LOGGER	East Bay	A4031K	10/15/1997		\$ 2,250.00	Good	Active
169936	Thermo 146i	DYNAMIC GAS CALIBRATOR	East Bay	1171160009	6/15/2017		\$ 13,580.59	Good	Active
172238	Thermo 1405	TEOM PM MONITOR	Gandy	1405A240991803	4/9/2018		\$ 20,565.75	Good	Active
0173578	Thermo 49IQ	Ozone Analyzer	Gandy	1181870059	8/18/2018		\$ 12,838.68	Good	Active
0173579	Thermo 49IQ-PS	Ozone Calibrator	Gandy	1181870060	9/17/2018		\$ 16,684.75	Good	Active
105564	Agilaire 8832	DATA LOGGER	Gandy	A3123K	10/15/1997		\$ 2,250.00	Good	Active
	DIY	Zero Air System	Gandy	NA				Good	Active
161072	Thermo 1405	TEOM PM MONITOR	Gardinier Park	1405A229161408	10/20/2014		\$ 17,290.00	Good	Active
118149	Agilaire 8832	DATA LOGGER	Gardinier Park	A4030K	9/6/2001		\$ 6,080.00	Good	Active
	Tisch TE-1000	High Volume Sampler	Kenly	VFC P7539	6/3/2010			Good	Active
180376	Magee Scientific AE-33	Aethalometer	Munro Street	AE33-S08-01061	9/19/2020		\$ 26,032.50	Good	Active
180878	Thermo 48IQ-TLE	Carbon Monoxide Analyzer	Munro Street	1201717981	9/19/2020		\$ 20,646.39	Good	Active
180673	Teledyne-API T200UP	Nitrogen Dioxide Analyzer Trace Level	Munro Street	160	9/28/2020		\$ 22,474.20	Good	Active
175878	Teledyne-API T640	Continuous PM2.5	Munro Street	744	8/21/2019		\$ 24,053.00	Good	Active
	EPC3783	Ultrafine Particle Counter	Munro Street	3783205001	1/28/2021		\$ 30,145.00	Good	Active
155474	Teledyne-API T700U	DYNAMIC GAS CALIBRATOR	Munro Street	295/268	5/9/2012		\$ 12,775.61	Good	Active
162087	Teledyne-API 701H	Zero Air System	AMD Lab	114	5/11/2015		\$ 7,110.00	Good	Active
157299	Agilaire 8832	DATA LOGGER	Munro Street	A4646K	5/31/2013		\$ 9,690.00	Good	Active
	Tisch TE-1000	High Volume Sampler	Patent	VFC P7807	6/3/2010			Good	Active
142735	Thermo 49i	Ozone Analyzer	Simmons Park	0717722870	7/20/2007		\$ 7,092.77	Good	Active
	DIY	Zero Air System	Simmons Park	NA	2/21/2020			Good	Active
139231	Thermo 49i PS	Ozone Calibrator	Simmons Park	0619417393	6/29/2006		\$ 9,567.50	Good	Active
131960	Agilaire 8832	DATA LOGGER	Simmons Park	A3124K	11/13/2003		\$ 5,000.00	Good	Active
162086	Teledyne-API 701H	Zero Air System	Sydney	115	5/11/2015		\$ 7,110.00	Good	Active
	DIY	Zero Air System	Sydney	NA				Good	Active
161613	URG 3000N	Carbon Sampling System	Sydney	B1164	3/3/2015		\$ 13,026.77	Good	Active
	ERG Carbonyl Sampler	Carbonyl Sampling System	Sydney	C-18	Rotating			Good	Active
158964	Thermo 5014i	Continuous PM2.5 Beta	Sydney	13381008	2/24/2014		\$ 19,183.60	Good	Active
177915	Thermo 42i-Y	NO-DIF-NOT ANALYZER	Sydney	1200416205	4/10/2020		\$ 32,170.60	Good	Active
169938	Thermo 49i	Ozone Analyzer	Sydney	1171160008	5/11/2017		\$ 11,640.00	Good	Active
55972	General Metals PM10	Particulate Size Selective Inlet	Sydney	593	10/5/1988		\$ 1,980.00	Good	Active
87043	General Metals PM10	Particulate Size Selective Inlet	Sydney	597	10/5/1988		\$ 1,980.00	Good	Active
0169326	Thermo 2025i	PARTISOL SAMPLER PM10/PM2.5	Sydney	2025IW2 1164 1703	3/23/2017		\$ 18,430.75	Good	Active
0169293	Thermo 2025i	PARTISOL SAMPLER PM10/PM2.5	Sydney	2025IW2 1163 1703	3/23/2017		\$ 20,148.56	Good	Active
0169325	Thermo 2025i	PARTISOL SAMPLER PM10/PM2.5	Sydney	2025IW2 1151 1702	3/23/2017		\$ 20,148.56	Good	Active
	Tisch TE-1000	PUF Air Sampler	Sydney	11038				Good	Active
	Graseby TE-1000	PUF Air Sampler	Sydney	NA				Good	Active
150562	Thermo 43iTLE	SO2 Analyzer Trace	Sydney	0910735777	4/21/2009		\$ 11,448.30	Good	Active
	Met One SASS	Speciation Aerosol Sampling System	Sydney	U21047	1/13/2005			Good	Active
164406	Thermo 48i TLE	Carbon Monoxide Trace level	Sydney	1160990209	7/25/2016		\$ 17,149.70	Good	Active
162634	Thermo 49i PS	Ozone Calibrator	Sydney	1151660005	7/1/2015		\$ 12,587.00	Good	Active
157306	Teledyne-API T700U	Multi-gas Dilution Calibrator	Sydney	612/301	5/22/2013		\$ 16,178.80	Good	Active
157300	Agilaire 8832	DATA LOGGER	Sydney	A4645K	5/31/2013		\$ 9,690.00	Good	Active
176265	Agilaire 8872	DATA LOGGER	AMD Lab	945	9/25/2019		\$ 9,735.00	Good	Stand-by
176266	Agilaire 8872	DATA LOGGER	AMD Lab	946	9/25/2019		\$ 9,735.00	Good	Stand-by
176252	Teledyne T300U	CO Analyzer	AMD Lab	70310000473	9/17/2019		\$ 14,661.80	Good	Stand-by
175878	Teledyne-API T640	Continuous PM2.5	AMD Lab	658	8/21/2019		\$ 24,053.00	Good	Stand-by
175104	Thermo 43iQTL	SO2 Analyzer Trace	AMD Lab	1191032525	5/31/2019		\$ 20,030.02	Good	Stand-by
0173579	Thermo 49iQ-PS	Ozone Calibrator	AMD Lab	1201717982	9/17/2018		\$ 16,684.75	Good	Stand-by
174874	Teledyne-API 701	Zero Air System	AMD Lab	1612	2/29/2016		\$ 4,385.00	Good	Stand-by
162688	Agilaire 8872	DATA LOGGER	AMD Lab	478	9/3/2015		\$ 9,000.00	Good	Stand-by
162633	Thermo 49i	Ozone Analyzer	AMD Lab	1151660004	7/1/2015		\$ 9,139.00	Good	Stand-by
1577305	Teledyne-API 701H	Zero Air System	AMD Lab	678	5/29/2015		\$ 7,283.30	Good	Stand-by
158964	Thermo 5014i	Continuous PM2.5 Beta	AMD Lab	CM13181009	8/19/2014		\$ 19,183.60	Good	Stand-by
157306	Teledyne-API T700U	Multi-gas Dilution Calibrator	AMD Lab	525	5/22/2013		\$ 23,503.30	Good	Stand-by
	Thermo 2025i	PARTISOL SAMPLER	AMD Lab	2025i20611201	3/12/2012			Good	Stand-by
153251	Met One BAM1020	Beta Gauge System	AMD Lab	K18874	11/29/2010		\$ 16,612.50	Good	Stand-by
153252	Met One BAM1020	Beta Gauge System	AMD Lab	K18875	11/29/2010		\$ 16,612.50	Good	Stand-by
	URG 3000N	Carbon Sampling System	AMD Lab	3N-B0502				Good	Stand-by
139230	Thermo 49i	Ozone Analyzer	AMD Lab	0619417392	6/29/2006		\$ 7,077.00	Good	Stand-by
135869	Thermo 43CTLE	SO2 Analyzer Trace	AMD Lab	0509111179	6/30/2005		\$ 11,980.00	Good	Stand-by
130566	Thermo 146C	DYNAMIC GAS CALIBRATOR	AMD Lab	0401304577	1/29/2004		\$ 8,805.00	Good	Stand-by
169937	Thermo 49iPS	Ozone Calibrator	AMD Lab	1171160007	6/15/2017		\$ 15,400.00	Good	Stand-by
157303	M651	Ultrafine Particle Counter	AMD Lab	M651130402	5/22/2013		\$ 24,399.50	Good	Stand-by
157307	Teledyne T300U	Carbon Monoxide Trace level	AMD Lab	124	5/22/2013		\$ 12,578.10	Good	Stand-by
177914	Thermo 1405	TEOM PM MONITOR	AMD Lab	1405A246292003	4/9/2020		\$ 22,076.70	Good	Stand-by
157304	Teledyne 633	Aethalometer	AMD Lab	AE33-S01-0093	5/22/2013		\$ 20,292.80	Good	Stand-by

Sarasota County

Property /Identification #	Manufacturer and Model #	Description	Location	Serial No.	Acquisition Date	Age	Initial Cost	Condition	Status
40072708	Agilaire 8872	Data Logger	Bee Ridge Park	1044	8/25/2020	1	\$ 7,850.00	New	Operating
40072710	Agilaire 8872	Data Logger	Lido	1045	8/25/2020	1	\$ 7,850.00	New	Operating
40072709	Agilaire 8872	Data Logger	Paw Park	1046	8/25/2020	1	\$ 7,850.00	New	Operating
N/A	Davis Instruments	MET Sensor	Bee Ridge Park	190802N01	2019	2	\$ 650.00	New	Operating
40070908	Thermo 1405	Particulate Sampler	Jackson	1405A243141903	3/4/2019	2	\$ 21,550.28	New	Operating
N/A	Davis Instruments	MET Sensor	Jackson	190802N07	2019	2	\$ 650.00	New	Operating
N/A	Davis Instruments	MET Sensor	Paw Park	190802N04	2019	2	\$ 650.00	New	Operating
N/A	Davis Instruments	MET Sensor	Lido	180807N01	2018	3	\$ 650.00	Good	Operating
40070109	Thermo 49iQ	Ozone Analyzer	Paw Park	1182250001	9/26/2018	3	\$ 10,079.01	New	Testing
40070110	Thermo 49iQ-PS	Ozone Calibrator	Paw Park	1182250002	9/26/2018	3	\$ 13,922.65	New	Testing
40068789	Teledyne T640	Particulate Sampler	Bee Ridge Park	212	8/29/2017	4	\$ 21,000.00	Good	Operating
40068790	Shelter One	T640 Enclosure	Bee Ridge Park	N/A	9/30/2017	4	\$ 6,500.00	Good	Operating
40068125	Thermo 49i-PS	Lido		1171300029	6/28/2017	4	\$ 13,581.00	Good	Operating
40066774	Agilaire 8872	Data Logger	Bee Ridge Park	0542	3/16/2016	5	\$ 6,990.00	Good	Back Up
40067751	Thermo 49i	Ozone Analyzer	Lido	1162290005	9/30/2016	5	\$ 9,337.50	Good	Operating
40066771	Thermo 1405	Particulate Sampler	Paw Park	1405A233811512	1/27/2016	5	\$ 19,395.00	Good	Operating
40063935	Thermo 2025i	Particulate Sampler	Bee Ridge Park	2025I205681402	4/3/2014	7	\$ 15,620.00	Good	Back Up
40064631	Thermo 49i	Ozone Analyzer	Jackson	1426962861	9/11/2014	7	\$ 9,150.00	Good	Operating
40064630	Thermo 49i-PS	Ozone Calibrator	Jackson	1426962860	9/11/2014	7	\$ 12,490.00	Good	Operating
40064692	Agilaire 8872	Data Logger	Lido	0334	10/31/2014	7	\$ 6,990.00	Good	Back Up
40064632	Teledyne T701	Zero Air Generator	Paw Park	64	9/19/2014	7	\$ 4,375.00	Good	Back Up
40064691	Agilaire 8872	Data Logger	Paw Park	0335	10/31/2014	7	\$ 6,990.00	Good	Back Up
40064694	Thermo 2025i	Particulate Sampler	Tallahassee	2025I207091410	12/17/2014	7	\$ 15,620.00	Good	On-loan
40064690	Agilaire 8872	Data Logger	BOB	0333	11/21/2013	8	\$ 6,495.00	Good	Back Up
40063474	Agilaire 8872	Data Logger	Jackson	0184	11/21/2013	8	\$ 6,495.00	Good	Back Up
40062204	Teledyne T700	MultiGas Calibrator	Paw Park	670	6/5/2013	8	\$ 15,138.40	Good	Back Up
40062203	Teledyne T200	Nox Analyzer	Paw Park	776	6/5/2013	8	\$ 11,372.80	Good	Back Up
40060203	Teledyne 400e	Ozone Analyzer	BOB	2529	6/29/2010	11	\$ 7,035.00	Fair	Back Up
40060204	Teledyne 703e	Ozone Calibrator	BOB	276	6/29/2010	11	\$ 9,166.00	Fair	Back Up
40059326	Ektō Manufacturing Co.	TEOM Enclosure	BOB Office	42011	7/13/2010	11	\$ 6,338.00	Good	Back Up
40059491	Thermo 49i	Ozone Analyzer	Paw Park	CM09190034	6/25/2009	12	\$ 7,930.00	Fair	Operating
40059492	Thermo 49i-PS	Ozone Calibrator	Paw Park	0916736286	6/25/2009	12	\$ 11,550.00	Fair	Operating
40057912	Ektō Manufacturing Co.	TEOM Enclosure	Bee Ridge Park	38851	1/23/2008	13	\$ 5,632.63	Good	Back Up
40058795	Thermo TEOM 1405	Particulate Sampler	Jackson	1405A202460809	9/30/2008	13	\$ 18,911.00	Fair	Back Up
40056961	Thermo TEOM 1400	Particulate Sampler	Bee Ridge Park	140AB267800706	9/30/2007	14	\$ 19,637.50	Fair	Back Up
40052744	Thermo 111	Zero Air Generator	BOB	427408888	9/30/2004	17	\$ 2,970.00	Fair	Operating
40050210	Thermo 49C-PS	Ozone Analyzer	BOB	49CPS77959387	4/25/2003	18	\$ 9,030.00	Fair	Back Up
40050209	Thermo 49C	Ozone Calibrator	BOB	49C77958387	4/25/2003	18	\$ 7,060.00	Fair	Back Up
40051472	Thermo 111	Zero Air Generator	BOB	1110326802150	11/14/2003	18	\$ 4,198.23	Fair	Back Up
40051235	RM Young 05103VP	Wind Vane	Jackson	58191	9/30/2003	18	\$ 1,039.50	Fair	Back Up
40051233	RM Young 05103VP	Wind Vane	Lido	58043	9/30/2003	18	\$ 1,040.00	Fair	Back Up
40051234	RM Young 05103VP	Wind Vane	Paw Park	58190	9/30/2003	18	\$ 1,039.50	Fair	Back Up
30002827	Wells Cargo	Trailer	Paw Park	1WC200J1343051042	11/19/2003	18	\$ 12,306.00	Fair	Operating
30002430	Wells Cargo	10' Trailer	Jackson	1WC200D17Y3043740	11/1/2000	21	\$ 8,852.25	Fair	Operating
40038151	ESC 8816	Data Logger	BOB	1665	2/17/1998	23	\$ 2,250.00	Fair	Back Up