




Lakeland

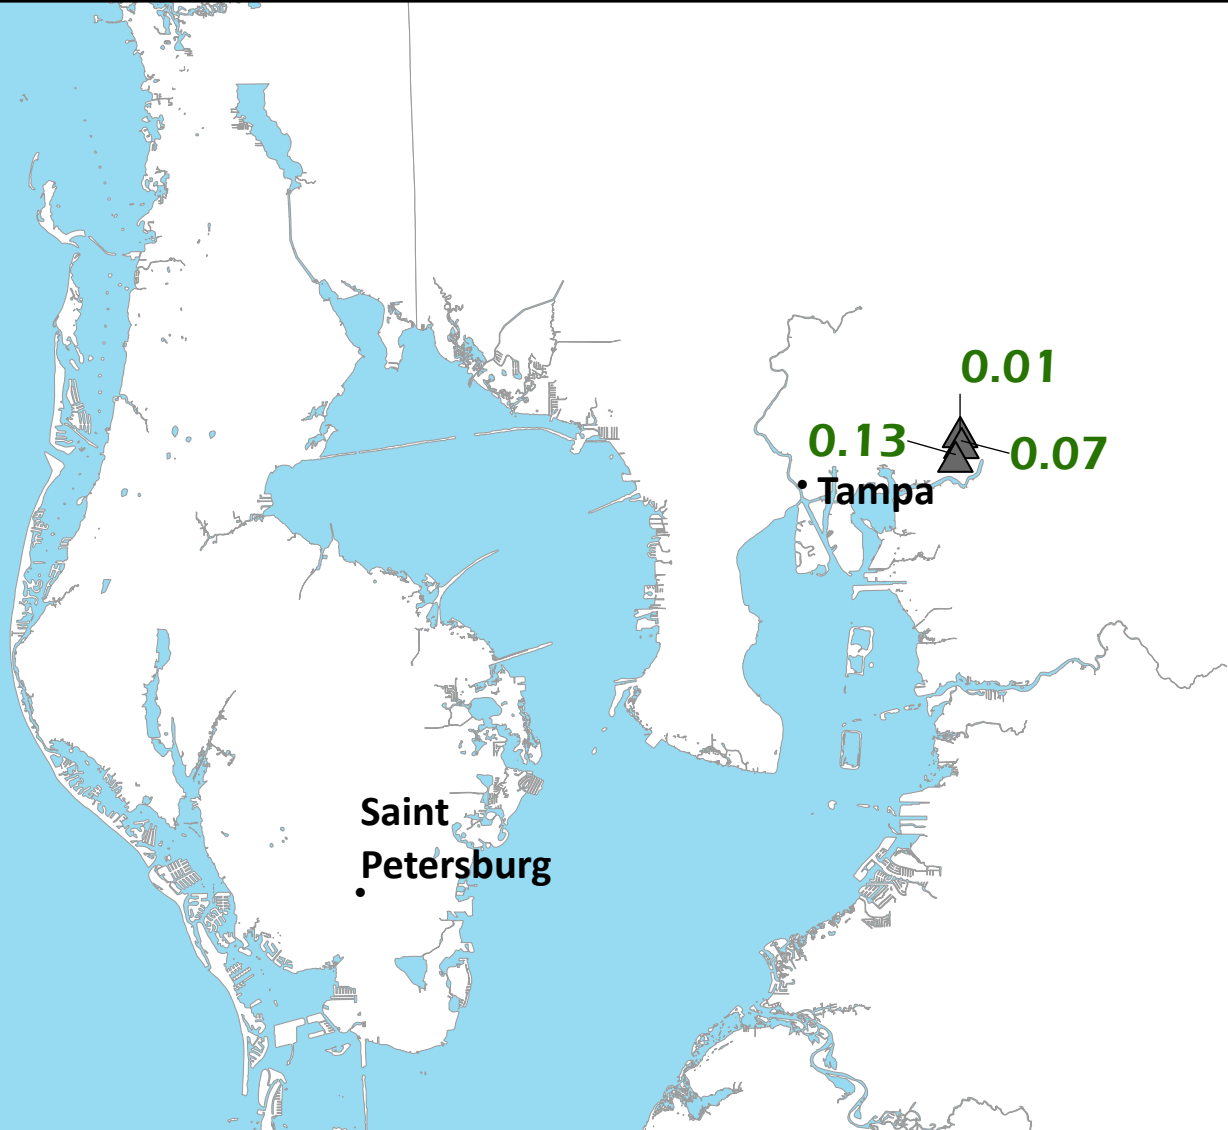

# 2017 - 2019 Monitored Design Values Lead - Pb

National Ambient Air Quality Standard:  
**0.15  $\mu\text{g}/\text{m}^3$**  3-Month Rolling Average Concentration ^  
**- All Florida Monitors in Compliance -**

^Design value is based on the maximum rolling 3-month average for the 38 month period beginning the last two months of the preceding year.

