




Lakeland

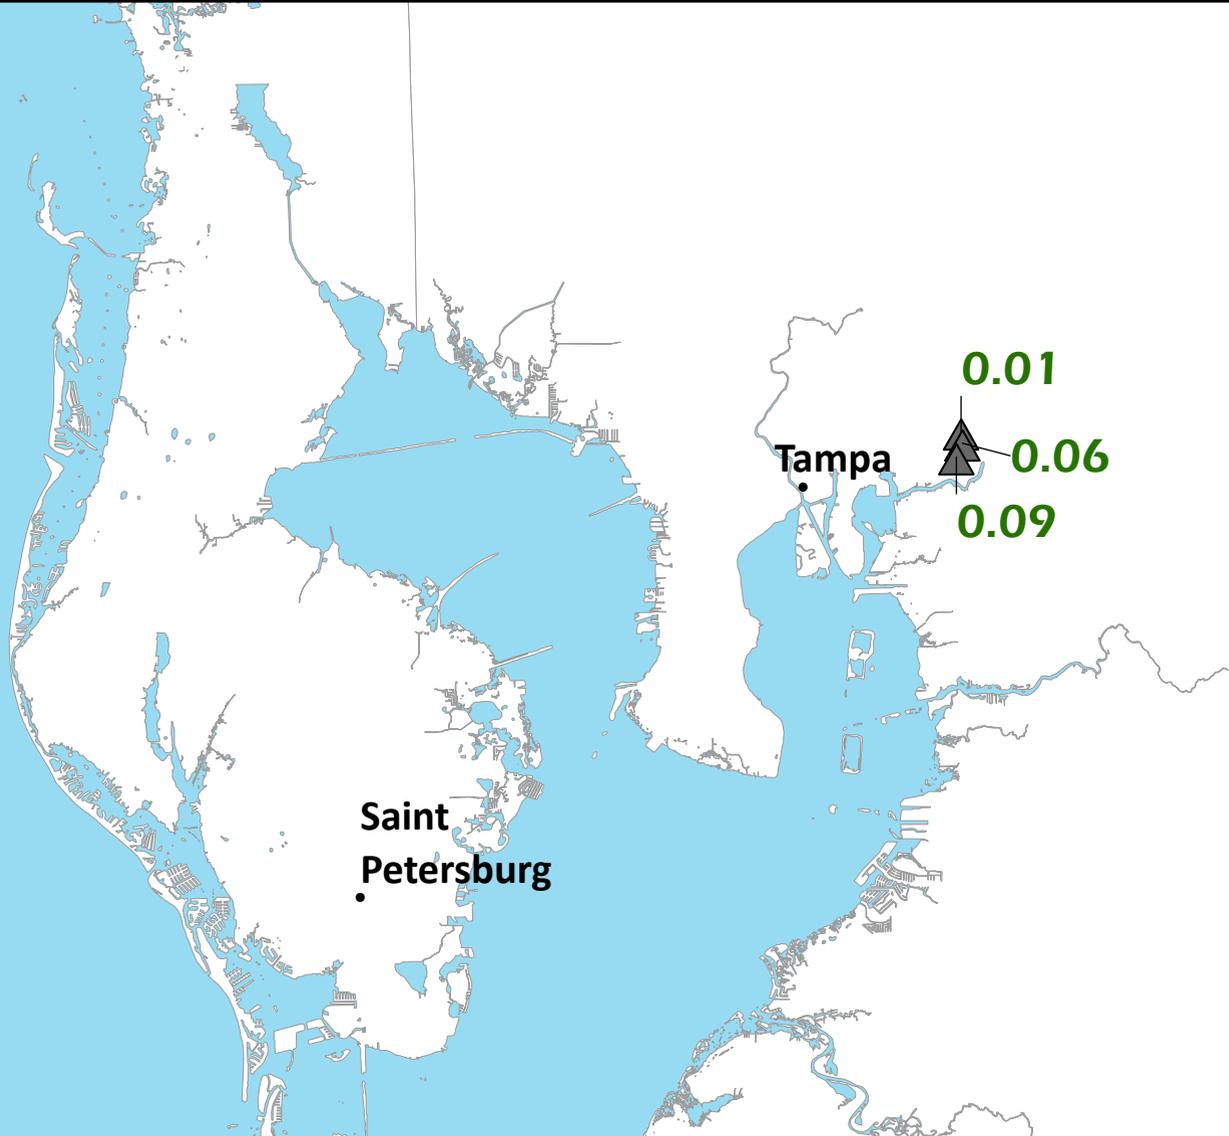

# 2019 - 2021 Monitored Design Values Lead - Pb

National Ambient Air Quality Standard:  
**0.15 µg/m<sup>3</sup>** 3-Month Rolling Average Concentration ^  
 - All Florida Monitors in Compliance -

^Design value is based on the maximum rolling 3-month average for the 38 month period beginning the last two months of the preceding year.

